


Laboratory Course

RWTH Aachen
University Münster

Neutron Scattering

Experiment Manual

Thomas Brückel, Dieter Richter, Georg Roth, Andreas Wischnewski
and Reiner Zorn (Editors)

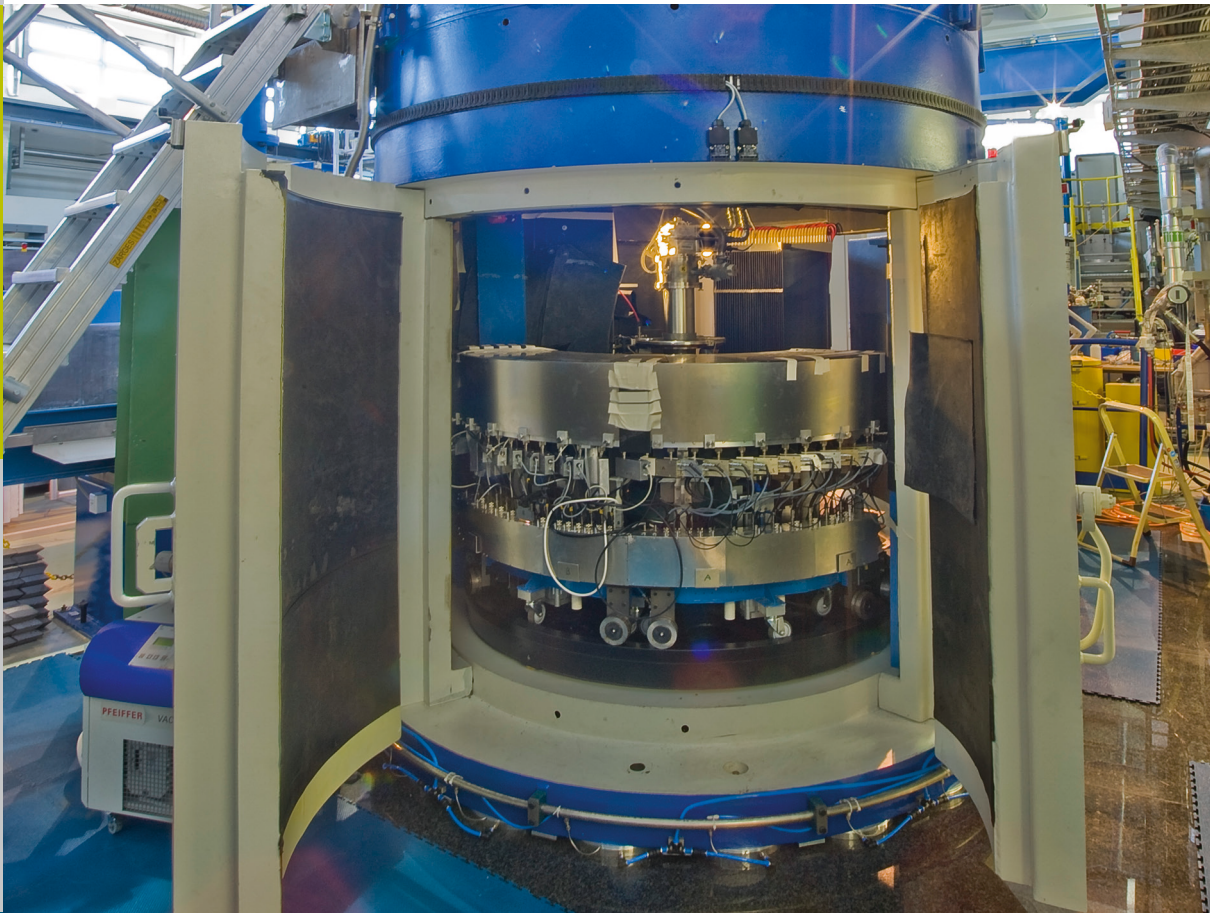

Schlüsseltechnologien /
Key Technologies
Band / Volume 107
ISBN 978-3-95806-056-2

Forschungszentrum Jülich GmbH
Jülich Centre For Neutron Science (JCNS)

Thomas Brückel, Dieter Richter, Georg Roth,
Andreas Wischnewski and Reiner Zorn (Editors)

Neutron Scattering

Experiment Manual of the JCNS Laboratory Course held at
Forschungszentrum Jülich and at the
Heinz Maier-Leibnitz Zentrum Garching
In cooperation with
RWTH Aachen and University of Münster

Bibliographic information published by the Deutsche Nationalbibliothek.
The Deutsche Nationalbibliothek lists this publication in the Deutsche
Nationalbibliografie; detailed bibliographic data are available in the
Internet at <http://dnb.d-nb.de>.

Publisher and
Distributor: Forschungszentrum Jülich GmbH
Zentralbibliothek
52425 Jülich
Phone +49 (0) 24 61 61-53 68 · Fax +49 (0) 24 61 61-61 03
e-mail: zb-publikation@fz-juelich.de
Internet: <http://www.fz-juelich.de/zb>

Cover Design: Grafische Medien, Forschungszentrum Jülich GmbH

Printer: Grafische Medien, Forschungszentrum Jülich GmbH

Copyright: Forschungszentrum Jülich 2015

Schriften des Forschungszentrums Jülich
Reihe Schlüsseltechnologien / Key Technologies Band / Volume 107

ISSN 1866-1807

ISBN 978-3-95806-056-2

The complete volume is freely available on the Internet on the Jülicher Open Access Server (JuSER)
at www.fz-juelich.de/zb/openaccess.

Neither this book nor any part of it may be reproduced or transmitted in any form or by any
means, electronic or mechanical, including photocopying, microfilming, and recording, or by any
information storage and retrieval system, without permission in writing from the publisher.

Contents


1	PUMA – Thermal Triple Axis Spectrometer	O. Sobolev, A. Teichert, N. Jünke
2	SPODI – High-resolution powder diffractometer	M. Hoelzel, A. Senyshyn, O. Dolotko, M. J. Mühlbauer
3	HEiDi – Hot Single Crystal Diffractometer for Structure Analysis with Neutrons	M. Meven
4	PANDA – Three-axis spectrometer	P. Link, A. Schneidewind
5	SPHERES – Backscattering spectrometer	J. Wuttke
6	DNS – Neutron Polarization Analysis	Y. Su
7	J-NSE – Neutron spin echo spectrometer	O. Holderer, O. Ivanova, M. Monkenbusch
8	KWS-1/-2 – Small Angle Neutron Scattering	H. Frielinghaus, M.-S. Appavou
9	KWS-3 – Very Small Angle Neutron Scattering Diffractometer with Focusing Mirror	V. Pipich
10	TREFF – Reflectometer	S. Mattauch, U. Rücker
11	TOFTOF – Time-of-flight spectrometer	L. Silvi, S. Busch, T. Unruh, W. Lohstroh

PUMA

Thermal Triple Axis Spectrometer

O. Sobolev, A. Teichert, N. Jünke

Forschungsneutronenquelle Heinz Maier-Leibnitz (FRM II)
Technische Universität München

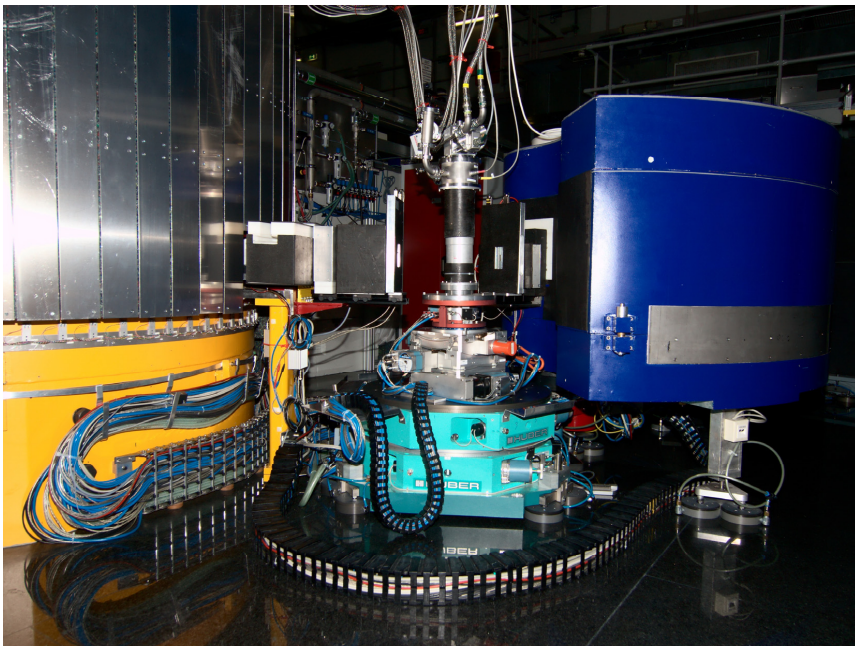

Contents

1	Introduction.....	3
2	Elastic scattering and Structure of Crystals	4
3	Inelastic Neutron Scattering and Phonons.....	5
4	Triple Axis Spectrometer PUMA.....	7
5	Experiment Procedure	9
6	Preparatory Exercises	12
7	Experiment-Related Exercises	12
	Useful formula and conversions.....	12
	References	13
	Contact	14


1. Introduction

Excitations in crystals can be described using formalism of dispersion relations of the normal modes or quasi-particles (phonons, magnons, etc.). These relations contain the most detailed information on the intermolecular interactions in solids.

The result of a neutron scattering experiment is the distribution of neutrons that have undergone an energy exchange $\hbar\omega = E_i - E_f$ and a wave vector transfer, $\mathbf{Q} = \mathbf{k}_i - \mathbf{k}_f$, after scattering by the sample.:

$$\frac{d^2\sigma}{d\Omega d\omega}(2\theta, \omega) = N \frac{k_f}{k_i} \left\{ \frac{\sigma_{coh}}{4\pi} S_{coh}(\mathbf{Q}, \omega) + \frac{\sigma_{inc}}{4\pi} S_{inc}(\mathbf{Q}, \omega) \right\} \quad (1)$$

σ_{coh} is coherent scattering cross section, σ_{inc} is incoherent scattering cross section. They are constants that can be found in tables (<http://www.ncnr.nist.gov/resources/n-lengths/>). $S(\mathbf{Q}, \omega)$ functions depend only on the structure and dynamics of the sample and do not depend on the interaction between neutrons and the sample. $S_{inc}(\mathbf{Q}, \omega)$ reflects individual motions of atoms. $S_{coh}(\mathbf{Q}, \omega)$ provides the information on the structure and collective excitations in the sample.

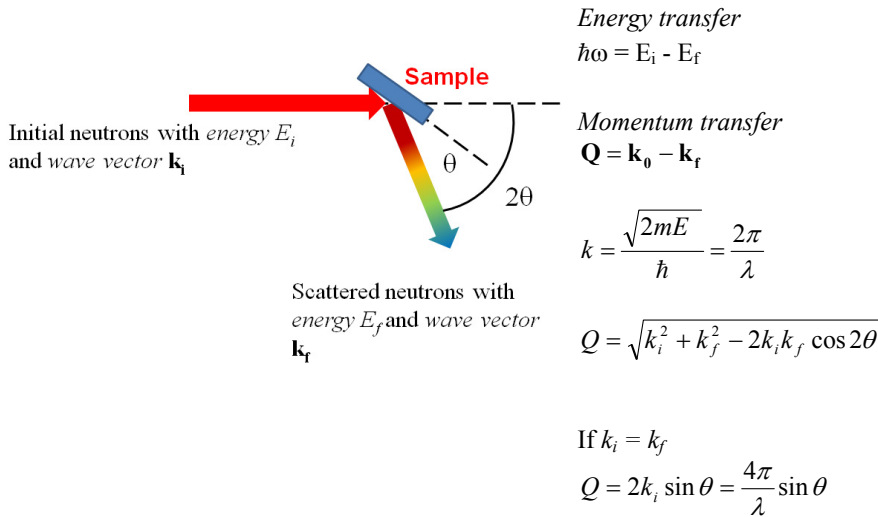

The triple axis spectrometer is designed for measuring the $S_{coh}(\mathbf{Q}, \omega)$ in monocrystals. Therefore this function is of special interest for us.

2. Elastic scattering and Structure of Crystals

In the case of coherent *elastic scattering*, when $\omega = 0$ ($k_i = k_f$) only neutrons, that fulfill the Brags law are scattered by the sample:

$$n\lambda = 2d_{hkl}\sin\theta_{hkl}, \quad (2)$$

where λ is a wavelength of neutron, d_{hkl} is a distance between crystal planes described by corresponding Miller indexes hkl . θ_{hkl} denotes the angle between incoming (outgoing) scattering beam and the (hkl) plane.

For the analysis of the scattering processes in crystals it is convenient to use the concept of the *reciprocal space*. For an infinite three dimensional lattice, defined by its primitive vectors \mathbf{a}_1 , \mathbf{a}_2 and \mathbf{a}_3 , its reciprocal lattice can be determined by generating three reciprocal primitive vectors, through the formulae:

$$\begin{aligned} \mathbf{g}_1 &= 2\pi \frac{\mathbf{a}_2 \times \mathbf{a}_3}{\mathbf{a}_1 \cdot \mathbf{a}_2 \times \mathbf{a}_3} \\ \mathbf{g}_2 &= 2\pi \frac{\mathbf{a}_1 \times \mathbf{a}_3}{\mathbf{a}_2 \cdot \mathbf{a}_1 \times \mathbf{a}_3} \\ \mathbf{g}_3 &= 2\pi \frac{\mathbf{a}_1 \times \mathbf{a}_2}{\mathbf{a}_3 \cdot \mathbf{a}_1 \times \mathbf{a}_2} \end{aligned} \quad (3)$$

Note the denominator is the scalar triple product. Geometrically, the scalar triple product $\mathbf{a}_1(\mathbf{a}_2 \times \mathbf{a}_3)$ is the volume of the parallelepiped defined by the three vectors.

Let us imagine the lattice of points given by the vectors \mathbf{g}_1 , \mathbf{g}_2 and \mathbf{g}_3 such that $\boldsymbol{\tau}$ is an arbitrary linear combination of these vectors:

$$\boldsymbol{\tau} = h\mathbf{g}_1 + k\mathbf{g}_2 + l\mathbf{g}_3, \quad (4)$$

where h, k, l are integers. Every point of the reciprocal lattice, characterized by $\boldsymbol{\tau}$ corresponds in the position space to the equidistant set of planes with Miller indices (h, k, l) perpendicular to the vector $\boldsymbol{\tau}$. These planes are separated by the distance

$$d_{hkl} = \frac{2\pi}{|\boldsymbol{\tau}_{hkl}|} \quad (6)$$

The Brag's condition for diffraction can be expressed in the following vector form:

$$\mathbf{Q} = \boldsymbol{\tau}_{hkl} \quad (7)$$

A useful construction for work with wave vectors in reciprocal space is the Brillouin zone (BZ). The BZ is the smallest unit in reciprocal space over which physical quantities such as phonon or electron dispersions repeat themselves. It is constructed by drawing vectors from one reciprocal lattice points to another and then constructing lines perpendicular to these vectors at the midpoints. The smallest enclosed volume is the BZ.

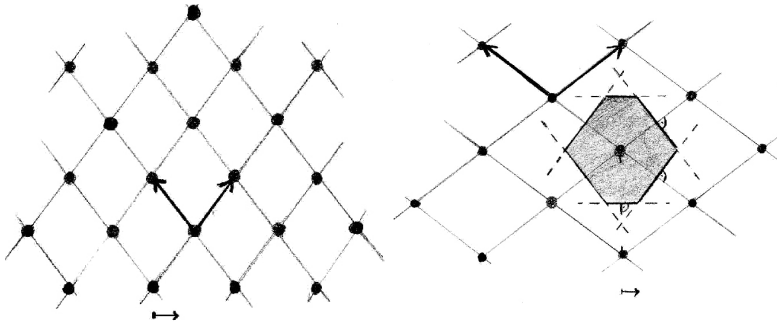


Fig.1 Real (left) and reciprocal (right) two dimensional lattices and BZ (gray area)

3. Inelastic Neutron Scattering and Phonons

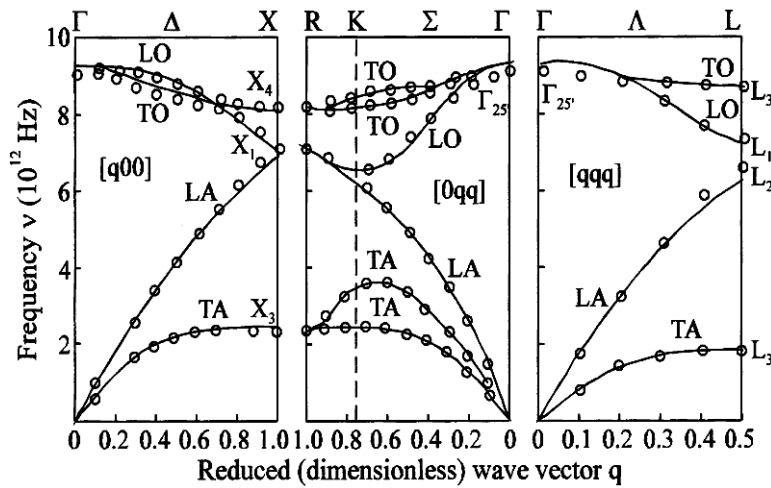


Fig.2 Phonon dispersion curves for Ge.

Atomic vibrations in a crystal can be analyzed in terms of lattice waves which are the normal modes of the crystal. The frequencies of normal modes ω are related to their wave vectors \mathbf{q} ($q = 2\pi/\lambda$) by the dispersion relations

$$\omega = \omega_j(\mathbf{q}), \quad (7)$$

where the index j denotes a particular branch. For a crystal with N atoms per primitive unit cell there are $3N$ branches of the frequency spectrum. Three branches are acoustic ones for which $\omega \rightarrow 0$ as $\mathbf{q} \rightarrow 0$; the other $3N-3$ are branches are optical branches for which ω tends to a finite value as $\mathbf{q} \rightarrow 0$. In certain directions of high symmetry the normal vibrations are strictly transverse or longitudinal. The energy quantum $\hbar\omega$ is called *phonon* in analogy to the phonon for electromagnetic waves.

If we want to measure the frequency of a phonon ω for a certain \mathbf{q} , the basic scattering conditions must fulfil the energy and momentum conservation laws:

$$E_i - E_f = \frac{\hbar}{2m_n}(k_i^2 - k_f^2) = \pm \hbar \omega(\mathbf{q}) \quad (9)$$

$$\mathbf{Q} = \mathbf{k}_i - \mathbf{k}_f = \mathbf{G} \pm \mathbf{q}$$

When the above conditions are fulfilled, the function $S_{coh}(\mathbf{Q}, \omega)$ shows a peak. We can held \mathbf{Q} constant and vary \mathbf{k}_i (\mathbf{k}_f) to measure intensity of scattered neutrons at different energy transfers. In order to keep \mathbf{Q} , and thus \mathbf{q} , constant while varying \mathbf{k}_i , the scattering angle must change as well as the relative orientation of the crystal with respect to \mathbf{k}_f .

The intensity of neutrons scattered by phonon is proportional to the square of the dynamical structure factor $F(\mathbf{Q})$:

$$S_{coh}(\mathbf{Q}, \omega) \sim |F(\mathbf{Q})|^2 = \left| \sum_{\kappa} b_{\kappa} \frac{\mathbf{Q} \cdot \mathbf{e}_{\kappa}(\mathbf{q}_j)}{\sqrt{m_{\kappa}}} \exp(-W_{\kappa}) \exp(-i\mathbf{q}\mathbf{r}_{\kappa}) \right|^2, \quad (10)$$

Where sum is taken over all atoms in unit cell with coordinates \mathbf{r}_{κ} , $\exp(-W)$ is a Debye-Waller factor, \mathbf{e}_{κ} denotes the polarization vector of the phonon. The scalar product $\mathbf{Q} \cdot \mathbf{e}_{\kappa}(\mathbf{q}_j)$ means that only lattice vibrations polarized along the momentum transfer are visible. This makes possible to distinguish transverse (TA) and longitudinal (LA) acoustic modes. For TA modes $\mathbf{e} \perp \mathbf{q}$, and therefore \mathbf{Q} must be perpendicular to \mathbf{q} , while for a LA mode, one must take $\mathbf{Q} \parallel \mathbf{q}$ (Fig. 3)

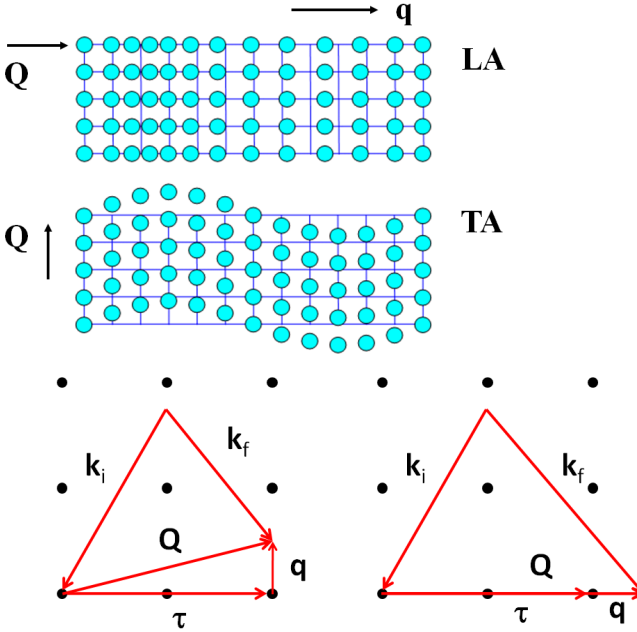


Fig. 3 Top: LA and TA phonons. Bottom: Neutron scattering diagram in the reciprocal space for TA (left) and LA phonons

4. Triple Axis Spectrometer PUMA

The three-axis instrument is the most versatile instrument for use in inelastic scattering because it allows one to probe nearly any coordinates in energy and momentum space in a precisely controlled manner. The three axes correspond to the axes of rotation of the *monochromator* (axis1), *the sample* (axis2), and *the analyzer* (axis3). The monochromator crystal selects neutrons with a certain energy from the white neutron beam emanating from the reactor. The monochromatic beam is then scattered off from the sample (second axis). The neutrons scattered by the sample can have a different energy from those incident on the sample. The energy of these scattered neutrons is then determined by the analyzer crystal (third axis). All three angles (θ_M , θ_S , θ_A) can vary during an experiment, the sample table and analyzer are equipped with air pads, so that they can glide over the “Tanzboden” (dancing floor). Below, we describe in detail each component of a triple-axis spectrometer.

Monochromator

A crystal monochromator is used to select neutrons with a specific wavelength. Neutrons with this wavelength interact with the sample and are scattered off at a similar (elastic) or different wavelength (inelastic). The energy of the neutrons both incident on and scattered from the sample is determined by Bragg reflection from the monochromator and analyzer crystals, respectively. For a specific Bragg plane (hkl) characterized by an interplanar spacing d_{hkl} , the crystal is rotated about a vertical axis. A pyrolytic graphite with $d_{002} = 3.35 \text{ \AA}$ (PG(002)) and a copper with $d_{220} = 1.28 \text{ \AA}$ (Cu(220)) monochromators are available at PUMA. The angular range of the monochromator $2\theta_M$ is of $15^\circ - 115^\circ$. The PG(002) is usually used for energies below 50meV ($\lambda > 1.3 \text{ \AA}$). For higher incident energies the Cu(220) can be used.

Sample table

The sample table from the company Huber provides a possibility to vary independently both $2\theta_S$ and θ_S . It is equipped with a goniometer moving the sample in the three translation axes x , y and z and tilting. The tilt angle is $\pm 15^\circ$. Single crystal experiments can be performed with an Euler cradle at PUMA. The sample environment includes magnets, pressure cells, cryostats and high temperature furnace.

Analyzer

Like the monochromator, the PG(002) analyzer consist of 20x5 separate analyzer crystal plates are mounted in an aluminum frame. There is an option to measure with the flat or horizontally and vertically focused analyser. The angular range of the analyser $2\theta_A$ is of $-130^\circ - 130^\circ$.

Detector and monitor

The detector consists of five counter tubes which are filled with a ^3He pressure of 5 bar. To be able to monitor the neutron flux incident on the sample, a low-efficiency neutron counter monitor is usually placed before the sample. Such a monitor is required so that flux variation caused by, for example, the reactor power fluctuations and the change in reflectivity of the monochromator with neutron wavelength can be automatically corrected for.

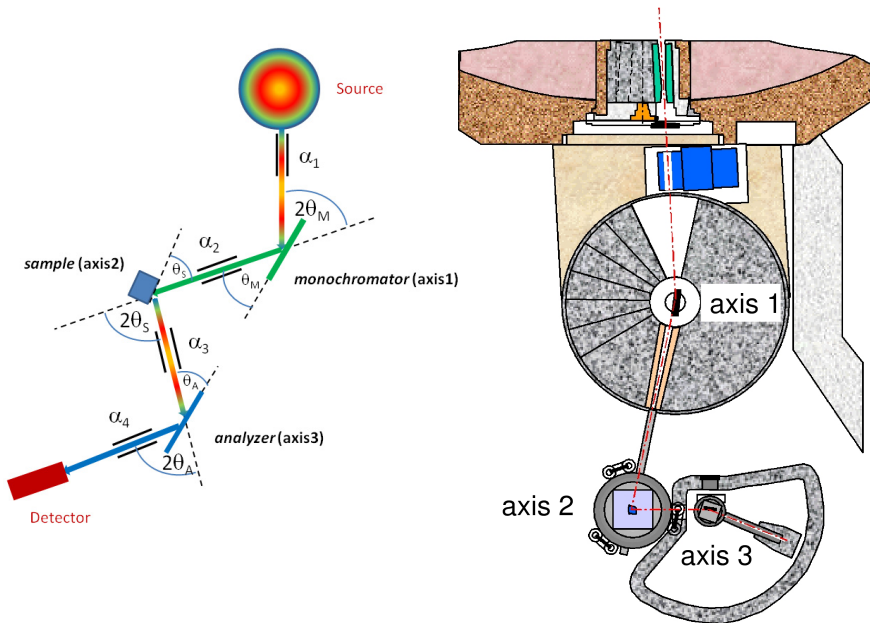


Fig.4 PUMA spectrometer.

Slits, Collimators, Filter

Additional components like slits or collimators are used to define the beam cross section. Collimators (α_1 - α_4) are used for the improvement of the resolution and to specify the beam divergence. They consist of multiple parallel arranged Gd_2O_3 coated foils with a defined angle to the beam. The angular divergence of the collimator in the horizontal plane α is defined by the distance between foils Δd and the length of the collimator l ($\tan \alpha = \Delta d / l$). Different collimators with a horizontal divergence between $10'$ and $60'$ are available at the instrument.

One of the problems of the TAS method is the possible presence of higher harmonics in the neutron beam. Higher harmonics arise from higher order (hkl) in Bragg's law (2). This means that if the monochromator (analyzer) crystal is set to reflect neutrons with a wavelength of λ from a given (hkl) plane, it will also reflect neutrons with wavelength λ/n . This leads to the appearance of several types of spurious peaks in the observed signal. Different filters are used to eliminate the high-order neutrons and to reduce the background. There are a sapphire filter (Al_2O_3) and an erbium filter (Er) at PUMA. They are installed in front of the monochromator. Sapphire filter is used wavelengths $\lambda > 1 \text{ \AA}$ and reduce the background inducing by the epithermal neutrons. Erbium filter is suitable as $\lambda/2$ filter for λ between 0.5 and 1 \AA as well as $\lambda/3$ filter for λ between 0.7 and 1.6 \AA .

Components	Axis	PUMAs notation	Description
Monochromator M	θ_M	meth	Monochromator Theta
	$2\theta_M$	mtt	Monochromator 2Theta
		mtx, mty	Monochromator Translation x-, y- direction
		mgx, mgy	Monochromator Goniometer x-, y- direction
		mfh, mfv	Monochromator Focus horizontal, vertical
Sample S	θ_S	psi	Sample Theta
	$2\theta_S$	phi	Sample 2Theta
		stx, sty, stz	Sample Translation x-, y-, z- direction
		sgx, sgy	Sample Goniometer x-, y- direction
Analyzer A	θ_A	ath	Analyzer Theta
	$2\theta_A$	att	Analyzer 2Theta
		atx, aty	Analyzer Translation x-, y- direction
		agx, agy	Analyzer Goniometer x-, y- direction
		afh	Analyzer Focus horizontal
Collimators		alpha1 – alpha4	Collimation

5. Experiment Procedure

The aim of the experiment is to measure acoustic phonons in a germanium sample. The phonons will be measured for [110] (LA) and [001] (TA) directions in [220] BZ. The experimental procedure shall contain the following steps:

Sample alignment

It is very difficult to align a sample with triple axis spectrometer, if the sample orientation is absolutely unknown. A sample must be pre-aligned, this means that the vertical axis of the sample must be known and roughly perpendicular to the ‘Tanzboden’. Then we shall do the following steps:

- Inform the control program of the spectrometer about a scattering plane of the sample. One must set two reciprocal vectors (in our case [110] and [001]) laying in the scattering plane.
- Drive spectrometer (θ_M , $2\theta_M$, θ_S , $2\theta_S$, θ_A , $2\theta_A$) to the position corresponding to [220] reflection.
- Scan θ_S and find the Brag’s peak.
- Scan corresponding goniometer axes to maximize intensity of the peak.
- Do the same for other reflection [004].
- Change the offset of the θ_S so that the nominal θ_S values correspond to intensity maxima for the above reflections.

Phonons measurements


For our measurements we will chose the const- k_f configuration with $k_f = 2.662 \text{ \AA}^{-1}$ ($E_f = 14.68 \text{ meV}$). This means that we will scan the energy transfer $\hbar\omega = E_i - E_f$ by varying incident energy $E_i(k_i)$. We are going to use PG(002) monochromator.

For LA phonon we will do constant-**Q** scans in the energy transfer range $\hbar\omega = 0 - 21$ meV (0 – 8 THz) for the following points:

Q(r.l.u.) = (2.1, 2.1, 0), (2.2, 2.2, 0), (2.3, 2.3, 0), (2.4, 2.4, 0), (2.5, 2.5, 0), (2.6, 2.6, 0), (2.7, 2.7, 0), (2.75, 2.75, 0).

For TA phonon we will do constant-**Q** scans in the energy transfer range $\hbar\omega = 0 - 15$ meV (0 – 3.6 THz) for the following points:


Q(r.l.u.) = (2, 2, 0.2), (2, 2, 0.3), (2, 2, 0.4), (2, 2, 0.5), (2, 2, 0.7), (2, 2, 0.8), (2, 2, 0.9), (2, 2, 1).

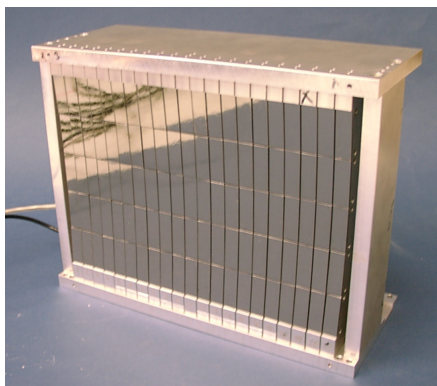

a) PG Analyzer



b) Soller collimator

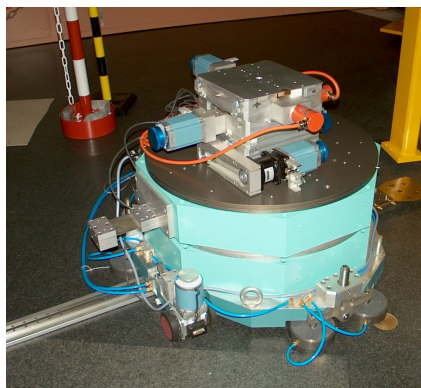


c) Sample table



d) Shutter, filters and collimators



e) Analyzer and Detector

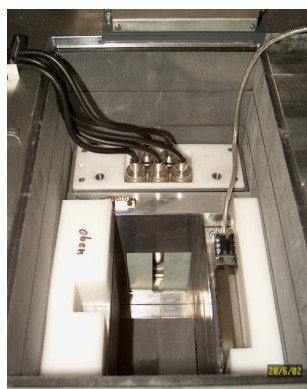f) Detector, consists of 5 ^3He tubes**Fig 5** Elements of PUMA

6. Preparatory Exercises

1. Calculate angles θ_M , $2\theta_M$, θ_S , $2\theta_S$ for the reflections [220] and [004] of *germanium* (cubic-diamond, $a = 5.66 \text{ \AA}$), supposing that $k_f = 2.662 \text{ \AA}^{-1} = \text{const}$, monochromator is PG(002), and check, if this reflections are measurable with our experimental setup.
2. Before doing a scan it is important to check that all point in $\mathbf{Q} - \hbar\omega$ space are available, instrument angles do not exceed high or low limits. Also, an experimental scientist must be sure that the moving instrument will not hit walls or any equipment. Calculate instrument parameters (θ_M , $2\theta_M$, θ_S , $2\theta_S$) for the momentum transfers $\mathbf{Q} \text{ (r.l.u.)} = (2.1, 2.1, 0)$, $(2.75, 2.75, 0)$ and energy transfers $\hbar\omega = 0$ and 21 meV . This can be done using an online triple-axis simulator:

<http://www.ill.eu/instruments-support/computing-for-science/cs-software/all-software/vtas/>

7. Experiment-Related Exercises

1. Plot obtained spectra for each \mathbf{Q} as a function of energy (THz). Fit the spectra with Gaussian function and find centers of the phopon peaks. The obtained phonon energies plot as a function of \mathbf{q} .
2. Why triple-axis spectrometer is the best instrument to study excitations in single crystals?
3. During this practicum we do not consider some problems that are very important for planning experiments with a triple axis instrument such as *resolution* and *intensity zones* [2]. Persons who have a strong interest to the triple-axis spectroscopy should study these topics by oneself. Advanced students should be able to explain our choice of Brillouin zone and parameters of scans for the phonon measurements.

Useful formula and conversions

$$1 \text{ THz} = 4.14 \text{ meV}$$

$$n\lambda = 2d_{hkl}\sin\theta_{hkl}$$

$$d_{hkl} = \frac{2\pi}{|\boldsymbol{\tau}_{hkl}|}$$

$$\mathbf{Q} = \mathbf{k}_0 - \mathbf{k}_f$$

$$Q = \sqrt{k_i^2 + k_f^2 - 2k_i k_f \cos 2\theta}$$

$$\text{If } k_i = k_f \text{ (elastic scattering) } Q = 2k_i \sin \theta = \frac{4\pi}{\lambda} \sin \theta$$

$$E [\text{meV}] = 2.072 \text{ k}^2 [\text{\AA}^{-1}]$$

References

- [1] Ch. Kittel, Einführung in die Festkörperphysik, Oldenburg, 14th ed., 2006
- [2] G. Shirane, S.M. Shapiro, J.M. Tranquada, Neutron Scattering with a Triple-Axis Spektrometer, Cambridge University Press, 2002
- [4] G. Eckold, P. Link, J. Neuhaus, Physica B, 276-278 (2000) 122- 123
- [5] B.N.Brockhouse and P.K. Iyengar, Physikal Review 111 (1958) 747-754
- [6] <http://www.ill.eu/instruments-support/computing-for-science/cs-software/all-software/vtas/>

Contact

PUMA

Phone: + 49 89 289 14914

Web: <http://www.mlz-garching.de/puma>

Oleg Sobolev

Georg-August Universität Göttingen

Institut für Physikalische Chemie

Aussenstelle am FRM II

Phone: + 49 89 289 14754

Email: oleg.sobolev@frm2.tum.de

Anke Teichert

Georg-August Universität Göttingen

Institut für Physikalische Chemie

Aussenstelle am FRM II

Phone: + 49 89 289 14756

Email: anke.teichert@frm2.tum.de

Jitae Park

Forschungsneutronenquelle Heinz Maier-Leibnitz

ZWE FRM II


Phone: + 49 89 289 13983

Email: jitae.park@frm2.tum.de

SPODI

High-resolution powder diffractometer

M. Hoelzel, A. Senyshyn, O. Dolotko, M.J. Mühlbauer
Forschungsneutronenquelle Heinz Maier-Leibnitz (FRM II)
Technische Universität München

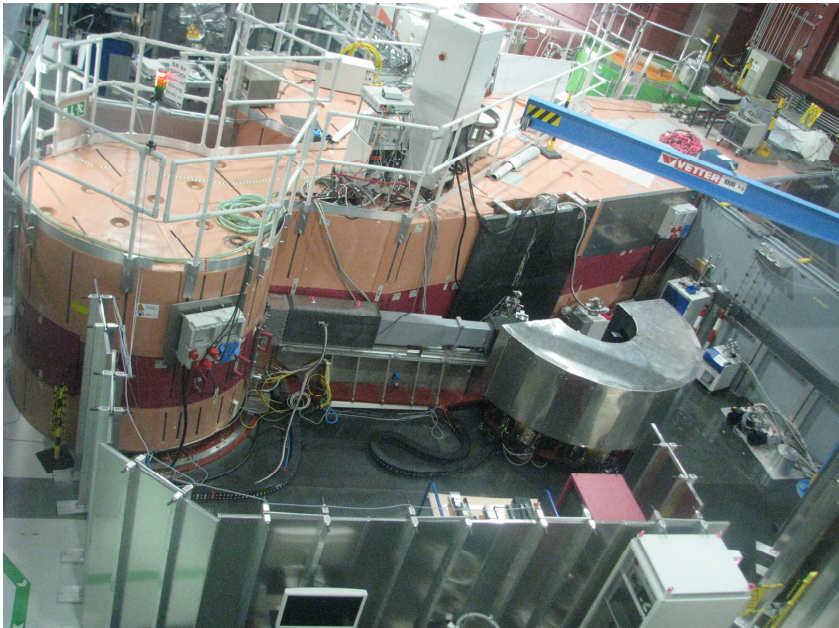

Contents

1	Applications of neutron powder diffraction.....	3
2	Basics of Powder Diffraction	4
3	Information from powder diffraction experiments.....	11
4	Evaluation of Powder Diffraction Data	13
5	Comparison between Neutron and X-ray diffraction	15
6	Setup of the high-resolution neutron powder diffractometer SPODI at FRM II	17
7	Experiment: Phase- and structure analysis of lead titanate at various temperatures	20
	References	23
	Contact	24

1. Applications of neutron powder diffraction

Powder diffraction reveals information on the phase composition of a sample and the structural details of the phases. In particular, the positions of the atoms (crystallographic structure) and the ordering of magnetic moments (magnetic structure) can be obtained. In addition to the structural parameters, also some information on the microstructure (crystallite sizes/microstrains) can be obtained. The knowledge of the structure is crucial to understand structure – properties – relationships in any material. Thus, neutron powder diffraction can provide valuable information for the optimisation of modern materials.

Typical applications:

Material	Task
Lithium-ion battery materials	Positions of Li atoms, structural changes/phase transitions at the electrodes during operation, diffusion pathways of Li atoms
Hydrogen storage materials	Positions of H atoms, phase transformations during hydrogen absorption/desorption
Ionic conductors for fuel cells	positions of O/N atoms, thermal displacement parameters of the atoms and disorder at different temperatures, diffusion pathways of O/N atoms
Shape memory alloys	stress-induced phase transformations, stress-induced texture development
materials with CMR effect	magnetic moment per atom at different temperatures
catalysers	Structural changes during the uptake of sorbents
Piezoelectric ceramics	Structural changes during poling in electric field, positions of O atoms
Nickel superalloys	Phase transformations at high temperatures, lattice mismatch of phases
magnetic shape memory alloys	Magneto-elastic effects, magnetic moment per atom at different temperatures and magnetic fields

2. Basics of Powder Diffraction

Diffraction can be regarded as detection of interference phenomena resulting from coherent elastic scattering of neutron waves from crystalline matter. Crystals can be imagined by a three-dimensional periodic arrangement of unit cells. The unit cell is characterised by the lattice parameters (dimensions and angles) and the positions of atoms or molecules. For diffraction experiments the probe should have a wavelength comparable to interatomic distances: this is possible for X-rays, electrons or neutrons.

Structure factor

The structure factor describes the intensity of Bragg reflections with Miller indexes (hkl) , based on the particular atomic arrangement in the unit cell

$$F_{hkl} = \sum_{j=1}^n b_j T_j \exp\{2\pi i \bar{H} \bar{R}_j\}$$

where

F_{hkl} : structure factor of Bragg reflection with Miller indexes hkl .

n : number of atoms in unit cell

b_j : scattering lengths (in case of neutron scattering) or atomic form factor (in case of X-ray diffraction) of atom j

T_j : Debye Waller factor of atom j

The scalar product $\bar{H} \bar{R}_j$ consists of the reciprocal lattice vector \bar{H} and the vector \bar{R}_j , revealing the fractional atomic coordinates of atom j in the unit cell.

$$\bar{H} \bar{R}_j = \begin{pmatrix} h \\ k \\ l \end{pmatrix} \cdot \begin{pmatrix} x_j \\ y_j \\ z_j \end{pmatrix} = hx_j + ky_j + lz_j$$

Thus, the structure factor can also be given as follows:

$$F_{hkl} = \sum_{j=1}^n b_j T_j \exp\{hx_j + ky_j + lz_j\}$$

The intensity of a Bragg reflection is proportional to the square of the absolute value of the structure factor: $I \propto |F_{hkl}|^2$

Debye-Waller Factor

The Debye-Waller Factor describes the decrease in the intensity of Bragg reflections due to atomic thermal vibrations.

$$T_j(Q) = \exp\left\{-\frac{1}{2}\langle(\vec{Q}\vec{u}_j)\rangle\right\}$$

vector \vec{u}_j reflects the thermal displacements of atom j

Braggs' Law

Braggs' Law provides a relation between distances of lattice planes with Miller indexes hkl , i.e. d_{hkl} , and the scattering angle 2θ of the corresponding Bragg peak. Braggs' law can be illustrated in a simplified picture of diffraction as reflection of neutron waves at lattice planes (figure 4). The waves which are reflected from different lattice planes do interfere. We get constructive interference, if the path difference between the reflected waves corresponds to an integer multiple of the wavelength.

The condition for constructive interference (= Braggs' law) is then:

$$2d_{hkl} \sin \theta = n\lambda$$

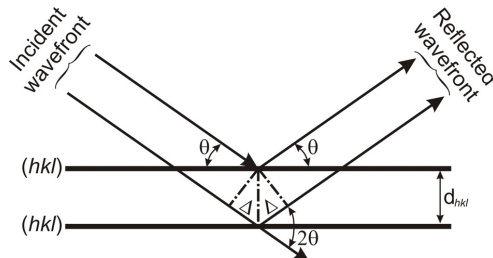


Figure 1: Illustration of Bragg's law: constructive interference of neutron waves, reflected from lattice planes, where θ , 2θ are Bragg angles, $2\Delta=2d_{hkl}\sin\theta$ is the path difference and $2\Delta=n\lambda$ is the constructive interference.

Applying Bragg's law one can derive the lattice spacings ("d-values") from the scattering angle positions of the Bragg peaks in a constant-wavelength diffraction experiment. With the help of d-values a qualitative phase analysis can be carried out.

Ewald's sphere

The Ewald's sphere provides a visualisation of diffraction with help of the reciprocal lattice. At first, we introduce the scattering vector \mathbf{Q} and the scattering triangle (Figure 2). The incident neutron wave is described by a propagation vector \mathbf{k}_i , the scattered wave is given by \mathbf{k}_f . In the case of elastic scattering (no energy transfer) both vectors \mathbf{k}_i and \mathbf{k}_f have the same length which is reciprocal to the wavelength.

$$|\mathbf{k}_i| = |\mathbf{k}_f| = \frac{2\pi}{\lambda}$$

remark:

The length of the wave vectors are sometimes given as $|\mathbf{k}_i| = |\mathbf{k}_f| = \frac{1}{\lambda}$ (This definition is found esp. in crystallographic literature, while the other one is more common for physicists).

The angle between vectors \mathbf{k}_i and \mathbf{k}_f is the scattering angle 2θ . The scattering vector \mathbf{Q} is the given by the difference between \mathbf{k}_i and \mathbf{k}_f :

$$\mathbf{Q} = \mathbf{k}_f - \mathbf{k}_i \quad |\mathbf{Q}| = 4\pi \frac{\sin \theta}{\lambda}$$

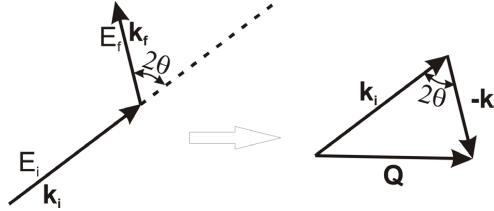


Figure 2: Illustration of scattering vector and scattering angle resulting from incident and scattered waves.

In the visualisation of the diffraction phenomena by Ewald the scattering triangle is implemented into the reciprocal lattice of the sample crystal – at first, we consider diffraction at a single crystal (Figure 3). Note that the end of the incident wave vector coincides with the origin of the reciprocal lattice. Ewald revealed the following condition for diffraction: we have diffraction in the direction of \mathbf{k}_f , if its end point (equivalently: the end point of scattering vector \mathbf{Q}) lies at a reciprocal lattice point hkl . All possible \mathbf{k}_f , which fulfil this condition, describe a sphere with radius $2\pi/\lambda$, the so called Ewald's sphere. Thus we obtain a hkl reflection if the reciprocal lattice point hkl is on the surface of the Ewald's sphere.

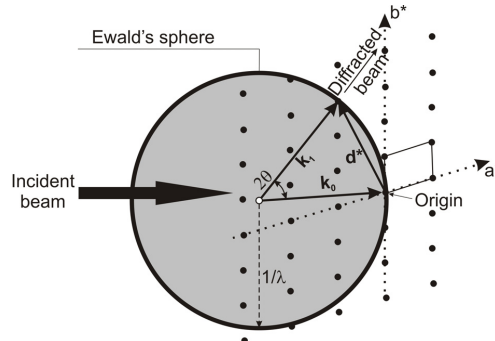


Figure 3: Illustration of diffraction using the Ewald's sphere.

Here, the radius of Ewald's sphere is given by $1/\lambda$ (For $|k_i| = \frac{2\pi}{\lambda}$ we obtain a radius of $2\pi/\lambda$).

We receive the following condition for diffraction: the scattering vector \vec{Q} should coincide with a reciprocal lattice vector \vec{H}_{hkl} ($\times 2\pi$):

$$\vec{Q} = 2\pi\vec{H}_{hkl}; \vec{H}_{hkl} = h\vec{a}^x + k\vec{b}^x + l\vec{c}^x; |\vec{H}_{hkl}| = d_{hkl}^x = \frac{1}{d_{hkl}}$$

From this diffraction condition based on the reciprocal lattice we can derive Bragg's law:

$$|\vec{Q}| = 2\pi|\vec{H}_{hkl}| \rightarrow 4\pi \frac{\sin \theta}{\lambda} = \frac{2\pi}{d_{hkl}} \rightarrow 2d_{hkl} \sin \theta = \lambda$$

The Ewald's sphere is a very important tool to visualize the method of single crystal diffraction: At a random orientation of a single crystalline sample a few reciprocal lattice points might match the surface of Ewald's sphere, thus fulfil the condition for diffraction. If we rotate the crystal, we rotate the reciprocal lattice with respect to the Ewald's sphere. Thus by a stepwise rotation of the crystal we receive corresponding reflections.

Powder Diffraction in Debye-Scherrer Geometry

In a polycrystalline sample or a powder sample we assume a random orientation of all crystallites. Correspondingly, we have a random orientation of the reciprocal lattices of the crystallites. The reciprocal lattice vectors for the same hkl , i.e. \mathbf{H}_{hkl} , describe a sphere around the origin of the reciprocal lattice. In the picture of Ewald's sphere we observe diffraction effect, if the surface of the Ewald's sphere intersects with the spheres of \mathbf{H}_{hkl} vectors. For a sufficient number of crystallites in the sample and a random distribution of grain orientations, the scattered wave vectors (\mathbf{k}_f) describe a cone with opening angle 2θ with respect to the incident beam \mathbf{k}_i .

In the so called Debye-Scherrer Geometry a monochromatic beam is scattered at a cylindrical sample. The scattered neutrons (or X-rays) are collected at a cylindrical detector in the scattering plane. The intersection between cones (scattered neutrons) and a cylinder (detector area) results in segments of rings (= Debye-Scherrer rings) on the detector. By integration of the data along the Debye-Scherrer rings one derives the conventional constant-wavelength powder diffraction pattern, i.e. intensity as a function of the scattering angle 2θ .

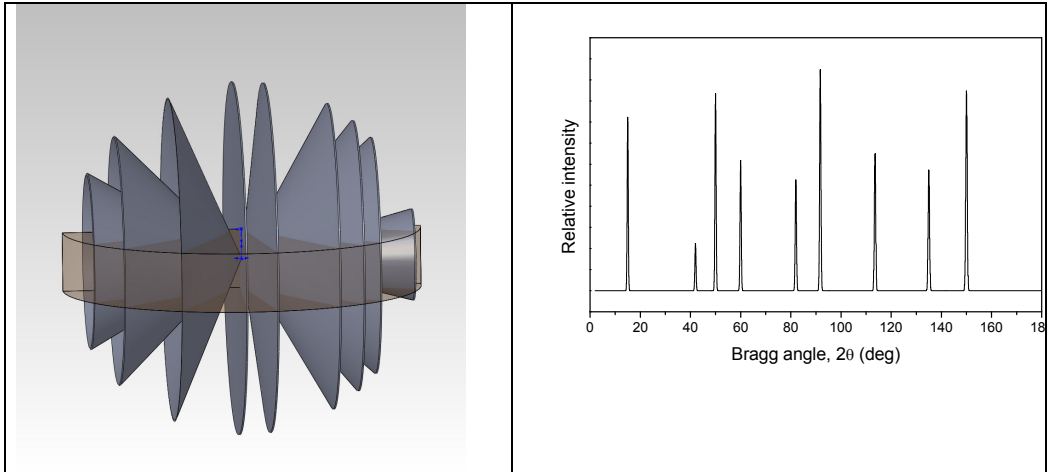


Figure 4: Illustration of powder diffraction in Debye-Scherrer Geometry. On the left: cones of neutrons scattered from a polycrystalline sample are detected in the scattering plane. On the right: resulting powder diffraction pattern.

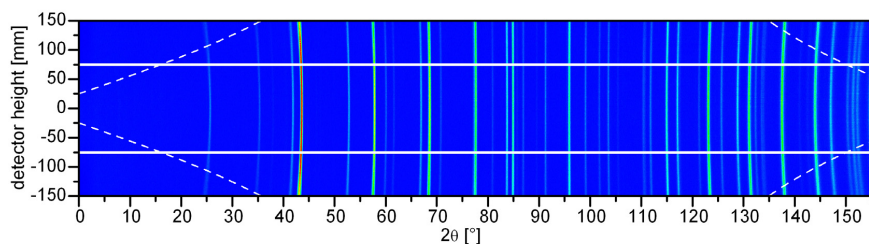


Figure 5: Two dimensional diffraction data (detector height vs. scattering angle 2θ), collected at high-resolution powder diffractometer SPODI, illustrating the Debye-Scherrer rings of a corundum sample.

Relations between Bragg positions and lattice parameters

With the help of Braggs law one can derive the lattice spacings “d-values” directly from the positions of Bragg reflections. The d-values are related with the lattice parameters of the unit cell (the cell dimensions a, b, c and the cell angles α, β, γ) and the Miller indexes (hkl) of the corresponding reflections. In the following, the relations are provided for the different crystal systems.

cubic
$$\frac{1}{d_{hkl}} = \frac{h^2 + k^2 + l^2}{a^2}$$

hexagonal
$$\frac{1}{d_{hkl}} = \frac{4}{3} \frac{h^2 + hk + k^2}{a^2} + \frac{l^2}{c^2}$$

tetragonal
$$\frac{1}{d_{hkl}} = \frac{h^2 + k^2}{a^2} + \frac{l^2}{c^2}$$

orthorhombic
$$\frac{1}{d_{hkl}} = \frac{h^2}{a^2} + \frac{k^2}{b^2} + \frac{l^2}{c^2}$$

monoclinic
$$\frac{1}{d_{hkl}} = \frac{h^2}{a^2 \sin^2 \beta} + \frac{k^2}{b^2} + \frac{l^2}{c^2 \sin^2 \beta} + \frac{2hl \cos \beta}{ac \sin^2 \beta}$$

3. Information from powder diffraction experiments

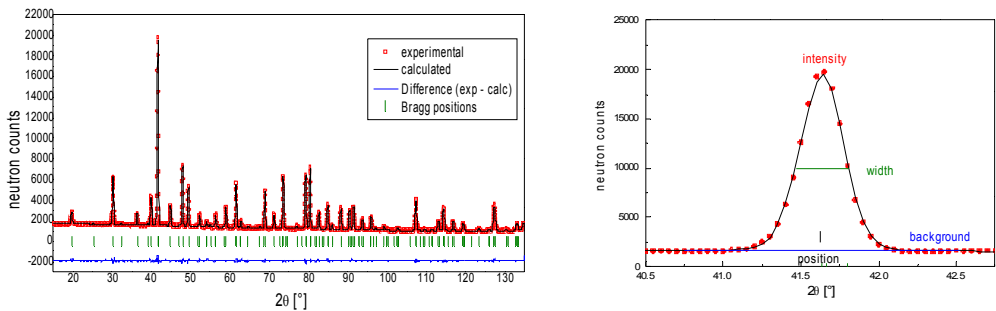


Figure 6: on the left: typical powder diffraction pattern. On the right: zoom on a single Bragg peak.

In the following, we will consider the information which can be derived from different elements of the diffraction patterns.

Positions (scattering angles) of Bragg reflections

- phase identification (from d-values)
- lattice parameters
- symmetry information (space group) by lattice parameters and selection rules (systematic extinction of reflections)

Intensity of Bragg reflections

- crystallographic structure
 - positions of atoms (fractional atomic coordinates)
 - occupancies of atoms on their sites
 - thermal displacement parameters
- magnetic structure
 - magnetic lattice (propagation vector)
 - magnetic symmetry (space group)
 - magnetic moment per atom
- quantitative phase analysis
- preferred orientation effects

Profiles of reflections

The reflection profiles result in a convolution of the instrumental resolution function with broadening effects of the sample

- microstructural information
 - microstrains
 - crystallite sizes

Modulation/Profile of Background

- short range order
- disorder
- amorphous contents

4. Evaluation of Powder Diffraction Data

The methods of data treatment can be classified in analysis of phase composition or phase transformation, structure solution and structure refinement.

Qualitative phase analysis is based on the determination of d-values and relative intensities (in particular intensities of strong reflections have to be considered). The phase identification is supported by crystallographic data bases (ICDD, ISCD), literature data and information from other methods (for instance, analysis of the chemical composition). Such kind of phase analysis is however typically carried out with X-ray diffraction.

The majority of neutron powder diffraction studies is based on experiments at various temperatures to investigate phase transformation behaviour as a function of temperature. There is an increasing demand for parametric studies, i.e. diffraction studies under various environmental conditions (temperature, electric or magnetic field, mechanical stress, gas atmosphere...) with particular attention to reaction pathways/reaction kinetics. This kind of investigations require in general high-intensity powder diffraction.

Powder diffraction data can be used either for phase identification or for the refinement of structural parameters, such as lattice parameters, fractional atomic coordinates, atomic occupancies and atomic displacement parameters by the full profile Rietveld analysis. In the Rietveld method, the full diffraction pattern is calculated by a structure model, taking into account the above mentioned structural parameters, as well as reflection profile parameters, instrumental parameters and background parameters. Using least-squares method, the experimental data can be fitted to the model in a stepwise refinement of the parameters. The complexity of the structures is directly dependent on the instrument specification, in particular, high-resolution powder diffractometers are designed for structure refinements on complex systems.

Besides structure refinement, also structure solution can be done based on powder diffraction patterns by various methods.

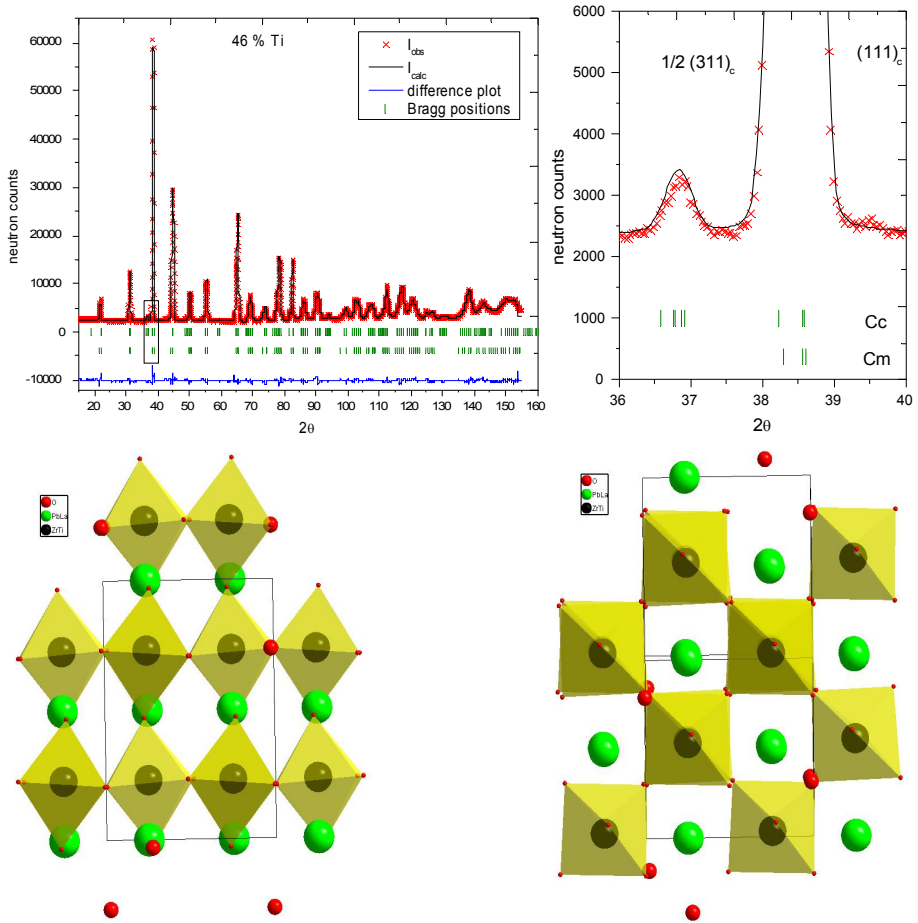


Figure 7: Data treatment of a measurement on the ferroelectric $\text{Pb}_{0.99}\text{La}_{0.01}\text{Zr}_{0.54}\text{Ti}_{0.46}\text{O}_3$, carried out at 5 K at diffractometer SPODI (FRM II): Diffraction pattern including experimental data, calculated data by Rietveld fit, Bragg reflection positions of the phases (space groups C_c and C_m) and difference plot (between experimental and calculated data). - zoom into the diffraction pattern, highlighting a superlattice reflection of the C_c phase. - structure model of the C_c phase, view in the $[001]_c$ direction - structure model of the C_c phase, view in the $[010]_c$ direction. In particular, the superstructure in the tiltings of oxygen octahedra can be seen.

5. Comparison between Neutron and X-ray diffraction

I) X-rays are scattered at electrons, neutrons are scattered at nuclei

In case of X-ray scattering, the scattering power of an atom (described by the atomic form factor f) is proportional to the number of electrons.

Neutrons are scattered at nuclei. Thus the interaction (described by the scattering length b) varies between different isotopes of an element. Scattering length of neighbouring elements in the periodic system can be very different.

implications:

Localisation of light elements next to heavier ones

X-ray diffraction is a powerful tool to determine the positions of heavy atoms, but the localisation of light atoms in the vicinity of much heavier atoms is often difficult or related with high uncertainties. Neutron diffraction is advantageous to localise light atoms such as H, D, Li, C, N, O.

Localisation of neighbouring elements in the periodic table

Neighbouring elements in the periodic table can hardly be distinguished by means of X-ray diffraction. Neutrons are advantageous for such cases: examples: Mn – Fe – Co – Ni or O – N.

Q-dependence of intensities

Since the size of electron clouds is comparable to the wavelength, the atomic form factor depends on $\sin\theta/\lambda$ or Q . Therefore the intensities of X-ray reflections decrease significantly for increasing Q (increasing scattering angles 2θ).

As the range of the neutron–nuclei–interaction is by orders of magnitude smaller than the wavelengths of thermal neutrons, scattering lengths do not depend on Q . As a consequence, neutron diffraction patterns do not show a decrease of Bragg reflection intensities for higher scattering angles, enabling the analysis of larger Q -ranges. In particular, neutron diffraction is advantageous for the analysis of thermal displacement parameters.

II) neutrons interact weakly with matter

implications:

sample volume

The flux from neutron sources much lower compared to X-ray tubes or even synchrotrons. In addition, neutrons interact weakly with matter. Therefore, much larger sample amounts are required compared to X-ray diffraction (“grams instead of milligrams”). On the other hand this weak interaction results in much higher penetration depths of neutrons, compared to laboratory X-ray diffractometers. Thus, polycrystalline bulk samples can be investigated. Furthermore, using large sample volumes avoids possible problems due to preferred orientation effects. In principle, bulk samples can also be investigated with high-energy synchrotron radiation. Anyhow in special cases the very low scattering angles related to low wavelength (in high-energy synchrotron studies) can cause difficulties.

Sample environments

The large penetration depths of neutrons facilitate the usage of sample environments like cryostat, furnaces, magnets... In general neutron scattering experiments are more powerful applying high or low temperatures. On the other hand, the small sample volume required for synchrotron studies gives better possibilities for high-pressure experiments.

III) neutrons exhibit a magnetic moment

Though neutrons do not have an electric charge, the internal charge distribution due to its three quarks along with the spin result in a magnetic moment of the neutron.

implications:

magnetic scattering

The interaction between the magnetic moment of the neutron and a possible magnetic moment of an atom results in a magnetic scattering contribution, incidentally in the same order of magnitude as the nuclear scattering contribution. The magnetic scattering contribution can be easily detected by means of neutron diffraction. In synchrotron diffraction studies, possible magnetic scattering events are by several orders of magnitude weaker than the Thomson scattering.

6. Setup of the high-resolution neutron powder diffractometer SPODI at FRM II

The main components of a constant-wavelength neutron powder diffractometer are: source, monochromator, sample and detector. Between these components collimation systems are installed which have high impact on the instrumental resolution function and the neutron flux.

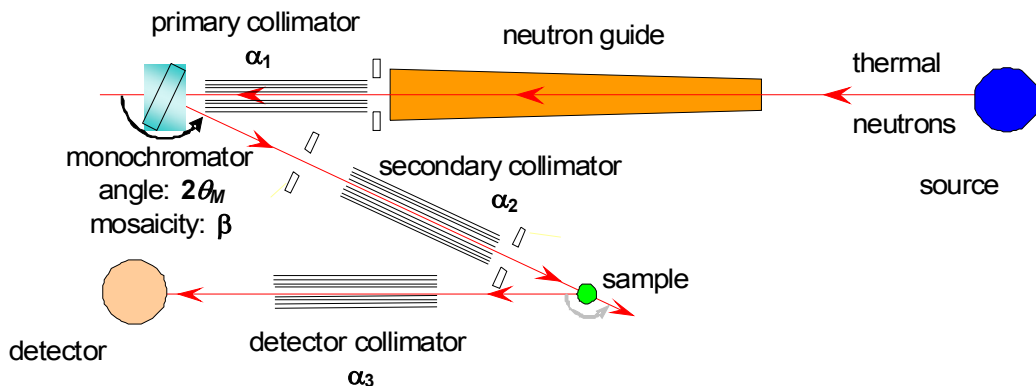


Figure 8: illustration of a typical instrumental layout, introducing the parameters used by Caglioti to describe the instrumental resolution function.

Instrumental resolution function

As shown by Caglioti, the instrumental resolution function of a constant-wavelength powder diffractometer can be approximated by:

$$FWHM = \sqrt{U \tan^2 \theta + V \tan \theta + W}$$

with the Caglioti parameters:

$$\begin{aligned}
 U &= \frac{4(\alpha_1^2 \alpha_2^2 + \alpha_1^2 \beta^2 + \alpha_2^2 \beta^2)}{\tan^2 \theta_m (\alpha_1^2 + \alpha_2^2 + 4\beta^2)} \\
 V &= \frac{-4\alpha_2^2 (\alpha_1^2 + 2\beta^2)}{\tan \theta_m (\alpha_1^2 + \alpha_2^2 + 4\beta^2)} \\
 W &= \frac{\alpha_1^2 \alpha_2^2 + \alpha_1^2 \alpha_3^2 + \alpha_2^2 \alpha_3^2 + 4\beta^2 (\alpha_2^2 + \alpha_3^2)}{(\alpha_1^2 + \alpha_2^2 + 4\beta^2)}
 \end{aligned}$$

in this approach it is assumed that all components have Gaussian transmission profiles. The resolution function is determined by the horizontal beam divergences $\alpha_1, \alpha_2, \alpha_3$, the monochromator angle $2\theta_m$ and the mosaicity of the monochromator β (Figure 8). As the impact of these parameters on the instrumental resolution function can be estimated, the Caglioti equations help to design an instrument to achieve a designated performance. However, it should be emphasised that in the approximations of Caglioti only the horizontal beam divergences are taken into account, neglecting vertical beam divergences by a vertical focusing monochromator or a vertical divergent neutron guide. Those effects are taken into account by ray-tracing methods, which allow a detailed modelling of the individual components.

The powder diffractometer SPODI has been designed to achieve both high resolution and good profile shape. In its standard configuration (highest resolution mode) SPODI uses a unique very high monochromator take-off angle of 155° along with a large monochromator-to-sample distance of 5 meters. An evacuated beam tube of about 4 m in length is located between the monochromator and the sample which also controls both vertical and horizontal neutron beam divergences at the sample position. Thus the natural neutron beam divergence in horizontal plane is $25'$ only. It can be reduced down to even $5'$ by optional Soller collimators in front of the sample.

Monochromator

At constant-wavelength diffractometers, the monochromatisation is performed using crystals followings Bragg's equation:

$$\begin{aligned}
 2d_{hkl} \sin \theta &= \lambda, \text{ where the effective transmission band is determined by a derivative} \\
 \frac{\Delta \lambda}{\lambda} &= \Delta \theta_M \cot \theta_M
 \end{aligned}$$

The width of the wavelength band $\Delta \lambda / \lambda$ strongly depends on the monochromator angle $2\theta_m$ and the mosaicity of the monochromator β , i.e $\Delta \theta_m$. Thus these parameters have a major impact on the instrumental resolution function and the flux on the sample.

Typically, the monochromator crystals are installed at a vertical focusing unit of 200 – 300 mm, allowing optimization of the intensity distribution at the sample position with respect to the monochromator – sample distance or the sample height. On the other hand, the vertical beam divergence results in a smearing of the Debye-Scherrer rings along the detector height (this effect depends also on the sample height). At the high-resolution powder diffractometer SPODI, 15 Germanium wafer-stack crystals with a (551)-orientation are used. Different wavelengths between 1.0 and 2.6 Å can easily be selected by rotation of the monochromator unit (without changing the monochromator take-off angle $2\theta_m$), i.e. by selecting different (*hkl*) reflection planes. In general, large wavelengths are advantageous to investigate structures exhibiting large d-values. This is the case for large unit cells, but in particular for magnetic ordering. With decreasing wavelengths, larger Q-values can be achieved. Thus, with lower wavelengths, more reflections can be observed in the same scattering angle range. Low wavelengths are in particular advantageous for the analysis of thermal displacement parameters or static disorder phenomena.

Detector array

At constant-wavelength diffractometers the data are collected in an angle-dispersive manner at equidistant 2θ points. Detector systems based on ^3He have been most commonly used due to their very high efficiency. Now, the world wide shortage of ^3He demands and promotes the development of alternatives, in particular scintillator based systems.

Classical high-resolution powder diffractometers, such as D2B (ILL), SPODI (FRM II), BT1 (NIST), ECHIDNA (ANSTO) use multidetector/multicollimator systems. The data are collected by ^3He tubes while the beam divergence is limited by Soller collimators. Such systems enable high Q-resolution over a broad scattering angle regime, while the resolution does not depend on the sample diameter. On the other hand, a multidetector concept requires a data collection by stepwise positioning of the detector array to collect the full diffraction pattern. Therefore, kinetic measurements are not feasible due to the fact that the sample must not change during the collection of a pattern.

The detector array of SPODI consists of 80 ^3He tubes, which are position sensitive in the vertical direction. Thus, two-dimensional raw data are obtained, which allow to rapid check for sample crystallinity, alignment and possible preferred orientation effects. The conventional diffraction patterns (intensity vs. scattering angle 2θ) are derived from the two-dimensional raw data by integration along the Debye-Scherrer rings.

7. Experiment: Phase- and structure analysis of lead titanate at various temperatures

samples

Lead zirconate titanates $\text{PbZr}_{1-x}\text{Ti}_x\text{O}_3$ („PZT“) exhibit piezo-, pyro- and ferroelectric properties. Piezoelectricity describes the generation of an electric polarisation as a consequence of a mechanical deformation – or the other way round the development of a macroscopic strain by an electric field. The crystallographic condition of piezoelectricity is the lack of an inversion center: as the balance points of negative and positive charge do not coincide the displacements of the ions in the electric field results in a polarization. Pyroelectricity refers to a spontaneous polarization of a material as a function of temperature. Ferroelectrics are special pyroelectric materials, in which the polarization can be switched by an electric field, resulting in a ferroelectric hysteresis.

The electromechanical properties of $\text{PbZr}_{1-x}\text{Ti}_x\text{O}_3$ can be understood by their phase transformation behaviour. At high temperatures they exhibit the perovskite structure with simple cubic symmetry (space group Pm-3m). Because of its symmetry (inversion center) this phase is not piezoelectric but paraelectric. During cooling, titanium-rich samples undergo a phase transition to a tetragonal phase (space group P4mm). This phase transformation is accompanied by atomic displacements. In particular, the $\text{Ti}^{4+}/\text{Zr}^{4+}$ are shifted in the opposite direction than O^{2-} ions, resulting in a dipole moment or a spontaneous polarisation. The material exhibits ferroelectric behaviour, with a polar axis in the direction of the pseudocubic c-axis, i.e. $[001]_c$. Zirconium rich samples undergo a phase transition towards a rhombohedral phase (space group R3m) during cooling. In this case, the atomic displacements result in a polar axis in direction $[111]_c$ with respect to the parent pseudocubic lattice. Materials $\text{PbZr}_{1-x}\text{Ti}_x\text{O}_3$ with compositions (Zr/Ti ratios) close to the so called morphotropic phase boundary between rhombohedral and tetragonal phase, show the highest piezoelectric response, i.e. the largest macroscopic strain as a function of the applied electric field. These compositions are therefore most interesting for technological applications. The piezoelectric properties can be modified further by adding doping elements to substitute Pb^{2+} or $\text{Ti}^{4+}/\text{Zr}^{4+}$ ions.

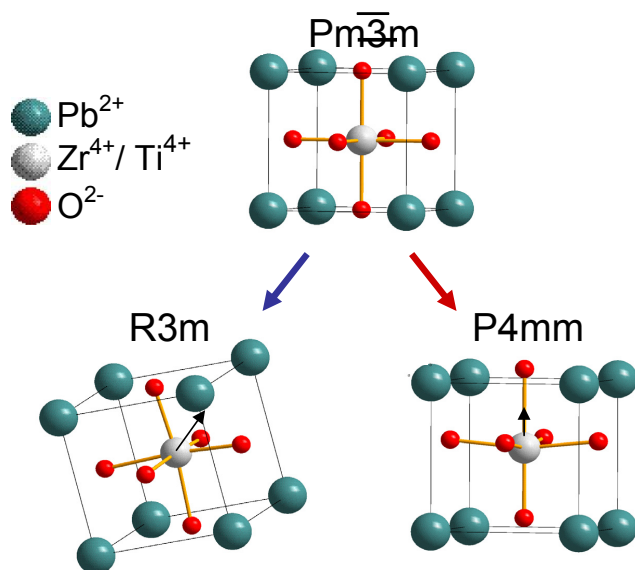


Figure 9: Structure models of the paraelectric cubic phase and the ferroelectric rhombohedral and tetragonal phases.

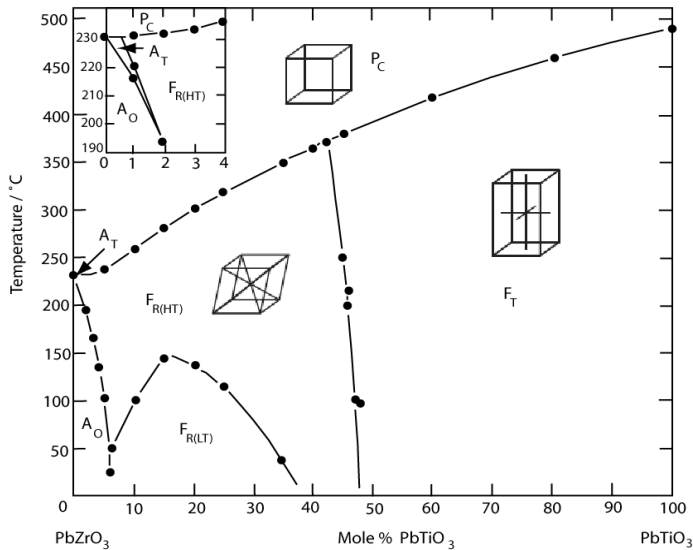


Figure 10: Phase diagram of $\text{PbZr}_{1-x}\text{Ti}_x\text{O}_3$, illustrating regions of phase stability for paraelectric cubic phase P_C , ferroelectric rhomboedral phases $F_{R(HT)}$ (= high temperature) and $F_{R(LT)}$ (= low temperature) and ferroelectric tetragonal phase F_T . From B. Jaffe, W. R. Cook, H. Jaffe, Piezoelectric Ceramics and Related Issues, Academic Press, London, 1971.

$\text{PbZr}_{1-x}\text{Ti}_x\text{O}_3$, find extensive applications

- transformation from mechanical in electric energy: ignition elements, lighters
- transformation from electric in mechanical energy (actuators): loudspeakers, sonar transducers, Active control of vibration
- transformation from mechanical force in an electric signal (sensors): strain gauges, microphones
- data storage, information technology: capacitors, F-RAM

Experiment

In the frame of the practical course, the temperature-dependent phase transformation behavior of a $\text{PbZr}_{1-x}\text{Ti}_x\text{O}_3$ with a composition on the tetragonal side should be investigated.

Diffraction patterns at different temperature steps between room temperature and 600 °C will be collected with a vacuum high-temperature furnace. The structural changes at different temperatures will be investigated by an analysis of the lattice parameters. Based on the experimental data, the relations between the structural changes and the corresponding physical properties can be discussed.

Following experimental procedures will be carried out

- sample preparation, filling the sample material into a sample can, adjustment of the sample stick, installation of the sample stick into the furnace
- short test measurement to check the sample adjustment and data quality
- editing a program to run the data collection at various temperatures and starting the scans
- data reduction: Derivation of diffraction patterns from the two-dimensional raw data
- data analysis: analysis of the lattice parameter changes as a function of temperature
- discussing the results with respect to structure – properties relationships

Literature

- [1] V. K. Pecharsky, P. Y. Zavalij, Fundamentals of Powder Diffraction and structural Characterisation of Materials (2003).
- [2] G. L. Squires, Introduction to the Theory of Thermal Neutron Scattering, Dover Reprints (1978).
- [3] C. Kittel, Einführung in die Festkörperphysik, 10. Edition, Oldenbourg (1993).
- [4] H. Dachs, Neutron Diffraction, Springer Verlag (1978).
- [5] H. Ibach und H. Lüth, Festkörperphysik, Einführung in die Grundlagen, 6. Edition, Springer Verlag (2002).
- [6] J.R.D. Copley, The Fundamentals of Neutron Powder Diffraction (2001), http://www.nist.gov/public_affairs/practiceguides/SP960-2.pdf.
- [7] A. D. Krawitz, Introduction to Diffraction in Materials Science and Engineering.
- [8] W. Kleber, Einführung in die Kristallographie, Oldenbourg (1998).

Contact

SPODI

Web: <http://www.mlz-garching.de/spodi>

Dr. Markus Hoelzel

Forschungsneutronenquelle Heinz Maier-Leibnitz (FRM II)
Technische Universität München

Phone: 089/289-14314

e-Mail: markus.hoelzel@frm2.tum.de

Dr. Anatoliy Senyshyn

Forschungsneutronenquelle Heinz Maier-Leibnitz (FRM II)
Technische Universität München

Phone: 089/289-14316

e-Mail: anatoliy.senyshyn@frm2.tum.de

Dr. Oleksandr Dolotko

Forschungsneutronenquelle Heinz Maier-Leibnitz (FRM II)
Technische Universität München

Phone: 089/289-14373

e-Mail: oleksandr.dolotko@frm2.tum.de

Dr. Martin J. Mühlbauer

Institut für Angewandte Materialien (IAM)
Karlsruher Institut für Technologie (KIT)

Phone: 089/289-14373


e-Mail: martin.muehlbauer@frm2.tum.de

HEiDi

Hot Single Crystal Diffractometer for Structure Analysis with Neutrons

M.Meven

Institut für Kristallographie, RWTH Aachen
and
Jülich Centre for Neutron Science
Forschungszentrum Jülich

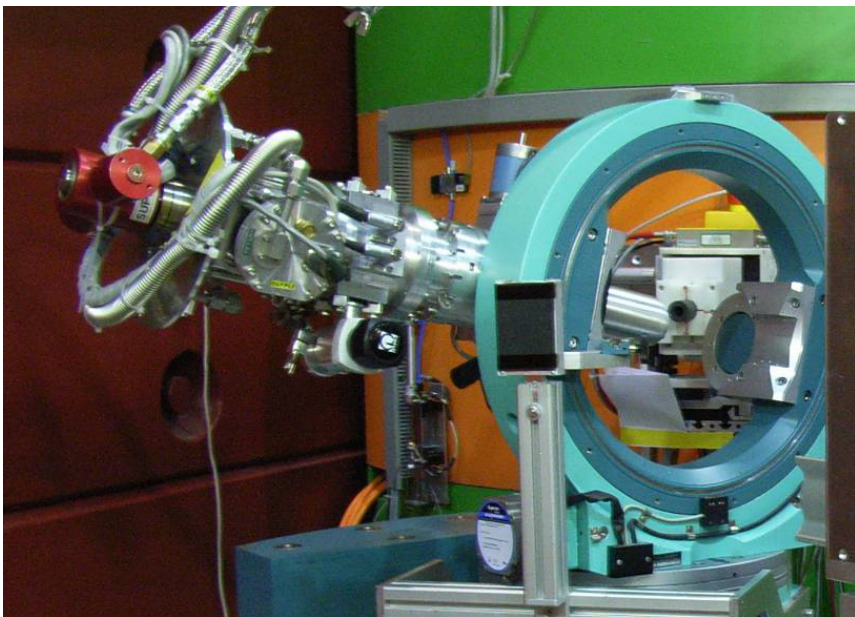

Contents

1	Introduction	3
2	Crystallographic Basics	3
3	Structure Determination with Diffraction.....	5
3.1	Introduction	5
3.2	Comparison of X-ray and Neutron Radiation.....	7
3.3	Special Effects	8
3.4	Summary of Theory of Method	10
3.5	From Measurement to Model	10
4	Sample Section.....	12
4.1	Introduction	12
4.2	Twinning.....	13
4.3	Oxygen Position	16
5	Preparatory Exercises.....	16
6	Experiment Procedure.....	17
6.1	The Instrument.....	17
6.2	Sequence of measurement in Theory.....	19
6.3	and in Practice	20
6.4	Data analysis.....	21
7	Experiment-Related Exercises	21
	References	22
	Contact	31

1 Introduction

Many properties of solid matter like their mechanical, thermal, optical, electrical and magnetic properties depend strongly on their atomic structure. Therefore, a good understanding of the physical properties needs not only the knowledge about the particles inside (atoms, ions, molecules) but also about their spatial arrangement. For most cases diffraction is *the* tool to answer questions about the atomic and/or magnetic structure of a system. Beyond this, neutron diffraction allows to answer questions where other techniques fail.

2 Crystallographic Basics

In the ideal case a complete solid matter consists of small identical units (same content, same size, same orientation like sugar pieces in a box). These units are called unit cells. A solid matter made of these cells is called a single crystal. The shape of a unit cell is equivalent to a parallelepiped that is defined by its base vectors \mathbf{a}_1 , \mathbf{a}_2 and \mathbf{a}_3 and that can be described by its lattice constants a , b , c ; α , β and γ (pic. 1). Typical lengths of the edges of such cells are between a few and a few ten Ångström ($1\text{\AA}=10^{-10}\text{ m}$). The combination of various restrictions of the lattice constants between $a \neq b \neq c$; $\alpha \neq \beta \neq \gamma \neq 90^\circ$ (triclinic) and $a = b = c$; $\alpha = \beta = \gamma = 90^\circ$ (cubic) yields seven crystal systems. The request to choose the system with the highest symmetry to describe the crystal structure yields fourteen Bravais lattices, seven primitive and seven centered lattices.

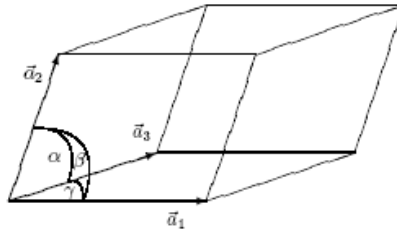


Fig. 1: Unit cell with $|\mathbf{a}_1|=a$, $|\mathbf{a}_2|=b$, $|\mathbf{a}_3|=c$, α , β , γ

Each unit cell contains one or more particles i . The referring atomic positions $\mathbf{x}_i = x_i \mathbf{a}_1 + y_i \mathbf{a}_2 + z_i \mathbf{a}_3$ are described in relative coordinates $0 \leq x_i, y_i, z_i < 1$. The application of different symmetry operations (mirrors, rotations, glide mirrors, screw axes) on the atoms in one cell yield the 230 different space groups (see [1]).

The description of a crystal using identical unit cells allows the representation as a three-dimensional lattice network. Each lattice point can be described as the lattice vector $\mathbf{t} = u \mathbf{a}_1 + v \mathbf{a}_2 + w \mathbf{a}_3$; $u, v, w \in \mathbf{Z}$. From this picture we get the central word for diffraction in crystals; the *lattice plane* or *diffraction plane*. The orientations of these planes in the crystal are described by the so called *Miller indices* h , k and l with $h, k, l \in \mathbf{Z}$ (see pic. 2). The reciprocal base vectors \mathbf{a}^*_1 , \mathbf{a}^*_2 , \mathbf{a}^*_3 create the reciprocal space with: $\mathbf{a}^*_i \cdot \mathbf{a}_j = \delta_{ij}$ with $\delta_{ij}=1$ for $i=j$ and $\delta_{ij}=0$ for $i \neq j$. Each point $\mathbf{Q} = h \mathbf{a}^*_1 + k \mathbf{a}^*_2 + l \mathbf{a}^*_3$ represents the normal vector of

a (hkl) Plane. Each plane cuts the crystal lattice along its base vectors \mathbf{a}_1 , \mathbf{a}_2 and \mathbf{a}_3 at $1/h*\mathbf{a}_1$, $1/k*\mathbf{a}_2$ and $1/l*\mathbf{a}_3$. A Miller index of zero means that the referring axis will be cut in infinity. Thus, the lattice plane is parallel to this axis.

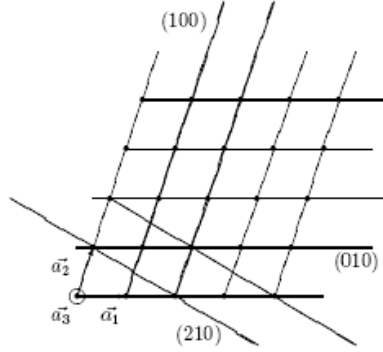


Fig. 2: Different lattice planes in a crystal lattice, \mathbf{a}_3 = viewing direction

The atoms in a unit cell are not rigidly fixed at their positions. They oscillate around their positions (e.g. thermal excitation). A simple description for this is the model of coupled springs. In this model atoms are connected via springs whose forces describe the binding forces between the atoms (e.g. van der Waals, Coulomb, valence). The back driving forces of the springs are proportional to the deviation x_i of the atoms from their mean positions and to the force constant D , thus. $F = -D*\Delta x$ (harmonic approximation).

Therefore, the atoms oscillate with $x_i = A_i*\sin(v*t)$ around their mean positions with the frequency v and the amplitude A_i . Both, v and A_i are influenced by the force constant D_j of the springs and the atomic masses m_i of the neighbouring atoms. The resulting lattice oscillations are called phonons in reference to the photons (light particles) in optics, which as well transport energy in dependence of their frequency. A more complex and detailed description of phonons in dependence on the lattice structure and the atomic reciprocal effects is given in lattice dynamics. In the harmonic approximation the displacements of an atom can be described with an oscillation ellipsoid. This ellipsoid describes the preferred spacial volume in which the atom is placed. Its so called mean square displacements (MSD) U_{jk}^i represent the different sizes of the ellipsoid along the different main directions j, k in the crystal. The simplest case is a sphere with the isotrope MSD B_i . In the next paragraph MSD are discussed from the point of view of diffraction analysis.

A full description of a single crystal contains information about lattice class, lattice constants and unit cell, space group and all atomic positions and their MSD. If the occupancy of one or more positions is not exactly 100%, e.g. for a mixed crystal or a crystal with deficiencies there has to be used also an occupancy factor.

3 Structure Determination with Diffraction

3.1 Introduction

Diffraction means coherent elastic scattering of a wave on a crystal. Because of the quantum mechanical wave/particle dualism x-rays as well as neutron beams offer the requested wave properties:

Electrons: $E = h\nu$; $\lambda = c/\nu$

Neutrons: $E_{\text{kin}} = 1/2 * m_n * v^2 = h\nu = p^2/2m_n$; $\lambda = h/p$; $p \sim \sqrt{(m_n k_B T)}$

h : Planck's constant; ν : oscillation frequency; λ : wavelength; c : light speed; p : impact; m_n : neutron mass; k_B : Boltzmann constant; T : temperature

Only the cross section partners are different (x-rays: scattering on the electron shell of the atoms, neutrons: core (and magnetic) scattering) as explained in detail below. In scattering experiments informations about structural properties are hidden in the scattering intensities I . In the following pages we will discuss only elastic scattering ($\lambda_{\text{in}} = \lambda_{\text{out}}$). The cross section of the radiation with the crystal lattice can be described as following:

Parallel waves of the incoming radiation with constant λ are diffracted by lattice planes which are ordered parallel with a constant distance of d . This is very similar to a light beam reflected by a mirror. The angle of the diffracted beam is equal to the angle of the incoming beam, thus the total angle between incoming and outgoing beam is 2Θ (see fig. 3).

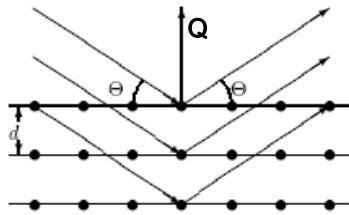


Fig. 3: Scattering on lattice planes

The overlap of all beams diffracted by a single lattice plane results in constructive interference only if the combination of the angle Θ , lattice plane distance d and wavelength λ meet Bragg's law:

$$2d \sin\Theta = \lambda$$

The largest distance $d_{hkl} = |\mathbf{Q}|$ of neighbored parallel lattice planes in a crystal is never larger than the largest lattice constant $d_{hkl} \leq \max(a; b; c)$. Therefore, it can only be a few Å or less. For a cubic unit cell ($a = b = c$; $\alpha = \beta = \gamma = 90^\circ$) this means:
 $d_{hkl} = a / \sqrt{(h^2 + k^2 + l^2)}$

With increasing scattering angle also the indices (hkl) increase while the lattice plane distances shrink with a lower limit of $d_{\text{min}} = \lambda/2$. Therefore, scattering experiments need

wavelengths λ in the same order of magnitude of the lattice constants or below. This is equal to x-ray energies of about 10 keV or neutron energies about 25 meV (thermal neutrons).

Ewald Construction: In reciprocal space each Bragg reflex is represented by a point $\mathbf{Q} = h^*\mathbf{a}_1^* + k^*\mathbf{a}_2^* + l^*\mathbf{a}_3^*$. A scattered beam with the wave vector \mathbf{k} fulfills Braggs law if the relationship $\mathbf{k} = \mathbf{k}_0 + \mathbf{Q}$, $|\mathbf{k}|=|\mathbf{k}_0|=1/\lambda$ is true, as shown in fig. 4. During an experiment the available reciprocal space can be described by an Ewald sphere with a diameter of $2/\lambda$ and the (000)-point as cross point of \mathbf{k}_0 direction and the centre of the diameter of the sphere. The rotation of the crystal lattice during the diffraction experiment is equal to a synchronous movement of the reciprocal lattice around the (000)-point. If Braggs law is fulfilled, one point ($h k l$) of the reciprocal lattices lies exactly on the Ewald sphere. The angle between the \mathbf{k} -vektor and the \mathbf{k}_0 -vektor is 2Θ . The limited radius of $1/\lambda$ of the Ewald sphere limits also the visibility of ($h k l$) reflections to $|\mathbf{Q}| < 2/\lambda$.

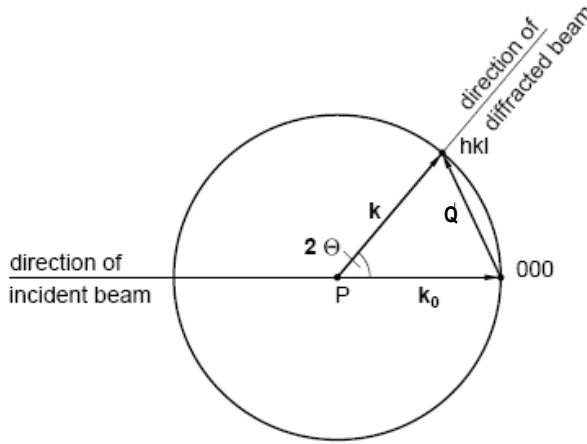


Fig. 4: Ewald construction

Determination of the Unit Cell: Following Braggs law the scattering angle 2Θ varies (for $\lambda=\text{const.}$) according to the lattice distance d_{hkl} . Thus for a given λ and known scattering angles 2Θ one can calculate the different d values of the different layers in the lattice of a crystal. With this knowledge it is possible to determine the lattice system and the lattice constants of the unit cell (although not always unambiguously!).

Atomic Positions in the Unit Cell: The outer shape of a unit cell does not tell anything about the atomic positions $\mathbf{x}_i=(x_i y_i z_i)$ of each atom in this cell. To determine the atomic positions one has to measure also the quantities of the different reflection intensities of a crystal. This works because of the relationship between the intensities of Bragg reflections and the specific cross section of the selected radiation with each element in a unit cell. Generally one can use the following formula for the intensity of a Bragg reflection ($h k l$) with \mathbf{Q} (kinetic scattering theory):

$$I_{hkl} \sim |F_{hkl}|^2 \text{ with } F_{hkl} = \sum_{i=1}^n s_i(\mathbf{Q}) \exp(2\pi i(hx_i + ky_i + lz_i))$$

The scattering factor F is a complex function describing the overlap of the scattering waves of each atom i (n per unit cell). $s_i(\mathbf{Q})$ describes the scattering strength of the i -th atom on its position \mathbf{x}_i in dependence of the scattering vector \mathbf{Q} , which depends on the character of cross section as described below.

In this context one remark concerning statistics: For measurements of radiation the statistical error σ is the square root of the number of measured events, e.g. x-ray or neutron particles. Thus, 100 events yield an error of 10% while 10,000 events yield an error of only 1%!

Mean Square Displacements (MSD): Thermal movement of atoms around their average positions reduce the Bragg intensities during a diffraction experiment. The cause for this effect is the reduced probability density and therefore reduced cross section probability at the average positions. For higher temperatures (above a few Kelvin) the MSD B_i of the atoms increase linearly to the temperature T , this means $B \sim T$. Near a temperature of 0 K the MSD become constant with values larger than zero (zero point oscillation of the quantum mechanical harmonic oscillator).

Thus, the true scattering capability s_i of the i -th atom in a structure has to be corrected by an angle-dependent factor (the so called Debye-Waller factor):

$$s_i(\mathbf{Q}) \rightarrow s_i(\mathbf{Q}) * \exp(-B_i(\sin \Theta / \lambda)^2)$$

This Debye-Waller factor decreases with increasing temperatures and yields an attenuation of the Bragg reflection intensities. At the same time this factor becomes significantly smaller with larger $\sin \Theta / \lambda \sim |\mathbf{Q}|$. Therefore, especially reflections with large indices loose a lot of intensity. The formula for anisotropic oscillations around their average positions looks like this:

$$s_i(\mathbf{Q}) \rightarrow s_i(\mathbf{Q}) * \exp(-2\pi^2(U_{11}^i h^2 a^{*2} + U_{22}^i k^2 b^{*2} + U_{33}^i l^2 c^{*2} + 2U_{13}^i hl a^*c^* + 2U_{12}^i hk a^*b^* + 2U_{23}^i kl b^*c^*))$$

The transformation between B and U_{eq} (from the U_{ij} calculated isotropic MSD for a sphere with identical volume) yields $B = 8\pi^2 U_{eq}$.

For some structures the experimentally determined MSD are significantly larger than from the harmonic calculations of the thermal movement of the atoms expected. Such deviations can have different reasons: Static local deformations like point defects, mixed compounds, anharmonic oscillations or double well potentials where two energetically equal atomic positions are very near to each other and therefore distribute the same atom over the crystal with a 50%/50% chance to one or the other position. In all those cases an additional contribution to the pure Debye-Waller factor can be found which yields an increased MSD. Therefore in the following text only the term MSD will be used to avoid misunderstandings.

3.2 Comparison of X-ray and Neutron Radiation

X-Ray Radiation interacts as electromagnetic radiation only with the electron density in a crystal. This means the shell electrons of the atoms as well as the chemical binding. The scattering capability s (atomic form factor $f(\sin \Theta / \lambda)$) of an atom depends on the number Z of its shell electrons ($f(\sin \Theta = 0) / \lambda = Z$). To be exact, $f(\sin \Theta) / \lambda$ is the Fourier transform of the radial electron density distribution $n_e(r)$: $f(\sin \Theta) / \lambda = s \int_0^\infty 4\pi^2 n_e(r) \sin(\mu r) / \mu r dr$ with $\mu = 4\pi \sin(\Theta) / \lambda$. Heavy atoms with many electrons contribute much stronger to reflection

intensities ($I \sim Z^2$) than light atoms with less electrons. The reason for the $\sin\Theta/\lambda$ -dependence of f is the diameter of the electron shell, which has the same order of magnitude as the wavelength λ . Because of this there is no pointlike scattering centre. Thus, for large scattering angles the atomic form factors vanish and also the reflection intensities relying on them. The atomic form factors are derived from theoretical spherical electron density functions (e. g. Hartree-Fock). The resulting $f(\sin\Theta/\lambda)$ -curves of all elements (separated for free atoms and ions) are listed in the international tables. Their analytical approximation can be described by seven coefficients ($c; a_i; b_i; 1 \leq i \leq 3$), see [1].

Neutron Radiation radiation interacts with the cores and the magnetic moments of atoms. The analogon to the x-ray form factor (the scattering length b) is therefore not only dependent on the element but the isotope. At the same time b -values of elements neighboured in the periodic table can differ significantly. Nevertheless, the scattering lengths do not differ around several orders of magnitude like in the case of the atomic form factors f . Therefore, in a compound with light and heavy atoms the heavy atoms do not dominate necessarily the Bragg intensities. Furthermore the core potential with a diameter about 10^{-15}\AA is a pointlike scattering centre and thus the scattering lengths b_n become independent of the Bragg angle and $\sin\Theta/\lambda$ respectively. This results in large intensities even at large scattering angles. The magnetic scattering lengths b_m can generate magnetic Bragg intensities comparable in their order of magnitude to the intensities of core scattering. On the other hand side the magnetic scattering lengths are strongly dependent on the $\sin\Theta/\lambda$ value due to the large spacial distribution of magnetic fields in a crystal. Therefore, it is easy to measure magnetic structures with neutrons and to separate them from the atomic structure.

Comparison: In summary in the same diffraction experiment the different character of x-ray and neutron radiation yield different pieces of information that can be combined. x-rays yield electron densities in a crystal while neutron scattering reveals the exact atomic positions. This fact is important because for polarised atoms the core position and the centre of gravity of electron densities are not identical any more. In compounds with light and heavy atoms structural changes driven by light elements need additional diffraction experiments with neutrons to reveal their influence and accurate atomic positions respectively. One has to take into account also that for x-rays intensities depend twice on $\sin\Theta/\lambda$. Once by the atomic form factor f , and twice by the temperature dependent Debye-Waller factor (see above). The first dependence vanishes if using neutron diffraction with $b=\text{const.}$ and decouples the structure factors from the influence of the MSD. In general this yields much more accurate MSD U_{ij} especially for the light atoms and might be helpful to reveal double well potentials.

3.3 Special Effects

From the relation $I \sim |F|^2$ one can derive that the scattering intensities of a homogenous illuminated sample increases with its volume. But there are other effects than MSD that can attenuate intensities. These effects can be absorption, extinction, polarization and the Lorentz factor:

Absorption can be described by the Lambert-Beer law:

$$I = I_0 \exp(-\mu x), \mu/\text{cm}^{-1} = \text{linear absorption coefficient, } x/\text{cm} = \text{mean path through sample}$$

The linear absorption coefficient is an isotropic property of matter and depends on the wavelength and kind of radiation. For x-rays penetration depths are only a few millimetre or below (e.g. for silicon with $\mu_{\text{MoK}\alpha}=1.546 \text{ mm}^{-1}$, $\mu_{\text{CuK}\alpha}=14.84 \text{ mm}^{-1}$ with penetration depths of 3 mm and 0.3 mm respectively). This limits transmission experiments to sample diameter of typically below 0.3 mm. To correct bias of intensities due to different scattering paths through the sample one has to measure accurately the sample size in all directions. Even for sphere like samples the mean path lengths depend on 2Θ ! In addition the sample environment must have an extraordinary small absorption

Thermal neutrons have for most elements a penetration depth of several centimeters. Thus, sample diameters of several millimeters and large and complex sample environments (furnaces, magnets, etc.) can be used. On the other hand side one needs sufficiently large samples for neutron diffraction which is often a delicate problem.

Extinction reduces also radiation intensities. But the character is completely different from that of absorption. In principle extinction can be explained quite easily by taking into account that each diffracted beam can be seen as a new primary beam for the neighbouring lattice planes. Therefore, the diffracted beam becomes partially backscattered towards the direction of the very first primary beam (Switch from kinetic to dynamic scattering theory!). Especially for very strong reflections this effect can reduce intensities dramatically (up to 50% and more). Condition for this effect is a merely perfect crystal.

Theoretical models which include a quantitative description of the extinction effect were developed from Zachariasen (1962) and Becker and Coppens [2, 3, 4, 5, 6]. These models base on an ideal spherical mosaic crystal with a very perfect single crystal (primary Extinction) or different mosaic blocks with almost perfect alignment (secondary Extinction) to describe the strength of the extinction effect. In addition, it is possible to take into account anisotropic extinction effect if the crystal quality is also anisotropic. Nowadays extinction correction is included in most refinement programs [7]. In general extinction is a problem of sample quality and size and therefore more commonly a problem for neutron diffraction and not so often for x-ray diffraction with much smaller samples and larger absorption.

Polarisation: X-ray radiation is electromagnetic radiation. Therefore, the primary beam of an x-ray tube is not polarized. The radiation hits the sample under a diffraction angle of Θ where it can be separated into two waves of same intensity, firstly with an electrical field vector parallel E_{\parallel} and secondly perpendicular E_{\perp} towards the Θ -axis. Whilst the radiation with E_{\parallel} will not be attenuated the radiation with E_{\perp} will be attenuated with $E_{\perp} \rightarrow \cos(2\Theta) E_{\perp}$. The polarization factor P for the attenuation has then the following formula ($I \sim E^2$):

$$P = (1 + \cos(2\Theta)^2)/2$$

Additional optical components like monochromator crystals also have an impact on the polarization and have to be taken into account accordingly.

Lorentz factor: The Lorentz factor L is a purely geometrical factor. It describes that during an ω - and Θ -scan respectively of Bragg reflections towards higher 2Θ values for the same angular speed $\Delta\omega/\Delta t$ an effectively elongated stay of the sample in the reflection position results.:

$$L = 1/\sin(2\Theta)$$

This has to be taken into account for any kind of radiation in an diffraction experiment.

3.4 Summary of Theory of Method

The different interactions of x-ray and neutron radiation with the atoms in a crystal make neutrons in general the better choice for a diffraction experiment. But on the other hand one has to take into account the available flux of x-rays and neutrons respectively. The flux of modern neutron sources like the Heinz Maier-Leibnitz neutron source (FRM II) is spread around a broad spectrum of neutron energies. In a sharp band of energies/wavelengths, e.g. $\Delta\lambda/\lambda < 10^{-3}$, there is the flux of neutrons several order of magnitude smaller than the flux of x-rays of a corresponding synchrotron source or x-ray tube in the laboratory. The reason for this is the fact that in an x-ray tube most x-rays are generated in a small energy band, the characteristic lines of the tube target (K_α , K_β , etc.). Additional metal foil used as filter allow to cut off unwanted characteristic lines which yields quasi monochromatic radiation of a single wavelength.

To use neutrons around a small energy band one has to use monochromator crystals. This reduces significantly the number of available neutrons for the diffraction experiment. Thus, the weak flux of neutrons and the weak cross section of neutrons with matter has to be compensated with large sample sizes of several millimeters. For the same reason the monochromatization of the neutrons is normally chosen to be not too sharp (resolution about $\Delta\lambda/\lambda \approx 10^{-2}$ for neutrons, $\Delta\lambda/\lambda \approx 10^{-5} - 10^{-6}$ for synchrotron).

3.5 From Measurement to Model

To get a structural model from the experimentally collected integral Bragg intensities one needs several steps in advance. Firstly one has to make sure that all reflections are measured properly (no shading, no $\lambda/2$ -contamination, no Umweganregung (Renninger-effect)). Damaged reflections have to be excluded from further treatment.

During data refinement not only the quantities of the relative intensities but also their errors are taken into account. The total statistical error σ of an integral intensity I_{obs} of a single reflection is calculated as following:

$$\sigma^2 = I_{\text{obs}} + I_{\text{background}} + (k I_{\text{total}})^2$$

The part $\sigma_0^2 = I_{\text{total}}$, $I_{\text{total}} = I_{\text{obs}} + I_{\text{background}}$ refers to the error caused by counting statistics. It contains as well the effective intensity I_{obs} as well as the contribution of the background. But there are other effects that influence the reproducibility of a measurement (and thus the total error), e.g. specific errors of the instrumental adjustment. Those errors are collected in the so called *McCandlish-Factor* k and contribute to the total error. Therefore, the total error cannot drop below the physically correct limit of the experiment and thus the impact of strong reflections does not become exaggerated in the refinement. The determination of k is done by measuring the same set of reflections several times during an experiment (the so called standard reflections). The mean variation of the averaged value represents k . In addition, the repeated measurement of standard reflections offers the opportunity to notice unwanted changes during experiment like structural changes or release from the sample holder.

To make sure the comparability of all reflections with each other, all intensities and errors are normalized to the same time of measurement (or monitor count rate) and undergo the Lorentz and (in the x-ray case) polarization correction.

Finally in advance of the data refinement there can be done an numerical (e.g. with DataP, [8]) or an empirical absorption if necessary. The quality of a measurement is checked in advance of the data refinement by comparing symmetry equivalent reflections and systematic extinctions to confirm the Laue group and space group symmetry. The result is written as internal R -value:

$$R_{\text{int}} = (\sum_{k=1}^m (\sum_{j=1}^{n_k} (<I_k> - I_j)^2)) / (\sum_{k=1}^m \sum_{j=1}^{n_k} I_j^2)_k$$

R_{int} represents the mean error of a single reflection j of a group k of n_k symmetry equivalent reflections, corresponding to its group and the total number m of all symmetrically independent groups. Therefore R_{int} is also a good mark to check the absorption correction. After these preliminary steps one can start the final data refinement.

At the beginning one has to develop a structural model. The problem with that is that we measure only the absolute values $|F_{hkl}|$ and not the complete structure factor $F_{hkl} = |F_{hkl}| \exp(i\phi)$ including its phase ϕ . Therefore, generally the direct Fourier transform of the reflection information F_{hkl} from reciprocal space into the density information ρ in the direct space (electron density for x-rays, probability density of atomic cores for neutrons) with

$$\rho(\mathbf{x}) \sim \sum_h \sum_k \sum_l F_{hkl} \exp(-2\pi(hx + ky + lz))$$

not possible. This can be done only by direct methods like Patterson, heavy atom method or anomalous dispersion for x-rays.

In the so called refinement program a given structural model (space group, lattice constants, atomic form factors, MSD, etc.) are compared with the experimental data and fitted. In a least squares routine those programs try to optimize (typically over several cycles) the free parameters to reduce the difference between the calculated structure factors F_{calc} and intensities $|F_{\text{calc}}|^2$ respectively and the experimentally found F_{obs} and $|F_{\text{obs}}|^2$ respectively. To quantize the quality of measurement there are several values in use:

$$1. \text{ unweighted } R\text{-value: } R_u = \sum_{hkl} |F_{\text{obs}}^2 - F_{\text{calc}}^2| / \sum_{hkl} F_{\text{obs}}^2$$

This value gives the alignment of the whole number of reflections without their specific errors.

$$2. \text{ weighted } R\text{-value: } R_w = (\sum_{hkl} w (F_{\text{obs}}^2 - F_{\text{calc}}^2)^2) / \sum_{hkl} w F_{\text{obs}}^4$$

This value represents the alignment of the whole number of reflections including their specific errors or weights ($w \sim 1/\sigma^2$). Sometimes weights are adopted in a way to suppress unwanted influence of the refinement algorithm by weak or badly defined reflections. Be aware that such corrections have to be done extremely carefully because otherwise the refinement adopts the data to the selected structural model and not the model to the experimental data!

$$3. \text{ Goodness of Fit } S: S^2 = (\sum_{hkl} w (F_{\text{obs}}^2 - F_{\text{calc}}^2)^2) / (n_{\text{hkl-reflections}} - n_{\text{free parameter}})$$

S should have a value near one if the weighting scheme and the structure model fit to the experimental data set.

4 Sample Section

4.1 Introduction

$\text{La}_{2-x}\text{Sr}_x\text{CuO}_4$ is one of the cuprate superconductors with K_2NiF_4 - structure for whose discovery the noble prize was granted in 1988 (Bednorz and Müller [9]). Pure La_2CuO_4 is an isolator. Doping with earth alcali metals (Ca^{2+} , Sr^{2+} , Ba^{2+}) on the La^{3+} lattice positions generates in dependence of the degree of doping superconductivity. Sr doping of $x=0.15$ yields a maximum T_c of 38 K.

Pure La_2CuO_4 undergoes at $T_{t-o}=530$ K a structural phase transition from the tetragonal high temperature phase (HTT)

$F4/mmm$: $a=b=5.384$ Å, $c=13.204$ Å, $\alpha=\beta=\gamma=90^\circ$ at $T=540$ K

to the orthorhombic low temperature phase (LTO)

$Abma$: $a=5.409$ Å, $b=5.357$ Å, $c=13.144$ Å, $\alpha=\beta=\gamma=90^\circ$ at room temperature.

The phase transition temperature T_{t-o} drops for $\text{La}_{2-x}\text{Sr}_x\text{CuO}_4$ with increased doping and disappears above $x=0.2$.

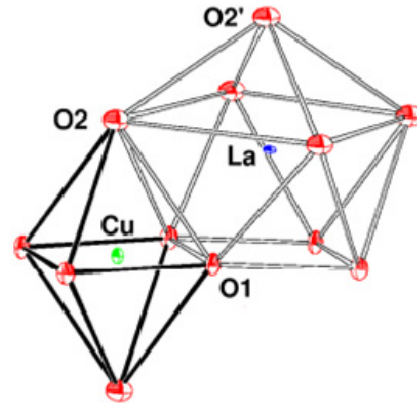
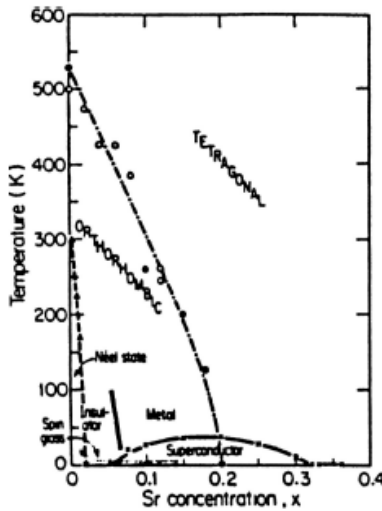


Fig.. 6 left: J. Birgenau, G. Shirane, HTC Superconductors I, World Scientific (1989)

Fig.. 6 right: Stuctural parts of La_2CuO_4 in the LTO phase

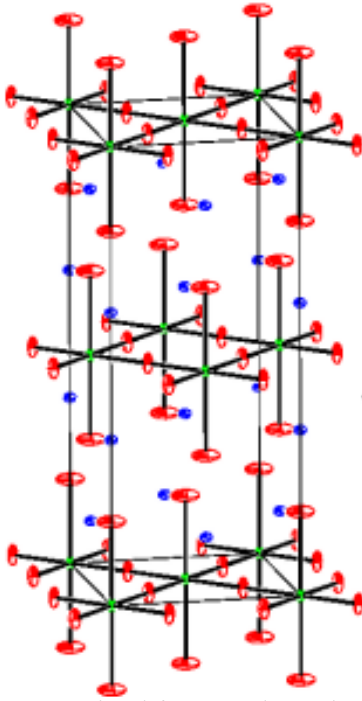


Fig. 7 left: tetragonal HTT phase

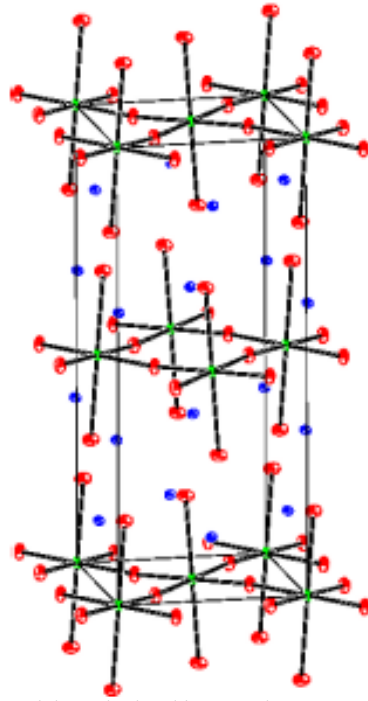


Fig. 7 right: orthorhombic LTO phase

4.2 Twinning

During the transition into the low temperature phase the CuO_6 octahedrons are tilted around their $[010]$ axis. Thus, the two axes of identical length in the HTT phase, a_1 and a_2 , are not equal in the LTO phase anymore. Instead, the longer one becomes the new a axis, the shorter one becomes the b axis. Whether a_1 or a_2 becomes the new a axis depends only on the real structure of the crystal, for instance grain boundaries or point defects. Therefore, one can find two equivalent crystallographic space groups in the LTO phase:

$Abma$ ($a_1 \rightarrow a, a_2 \rightarrow b$) and $Bmab$ ($a_1 \rightarrow b, a_2 \rightarrow a$)

For the structure factors in the LTO is valid:

$$F_{Abma}(hkl) = F_{Bmab}(khl)$$

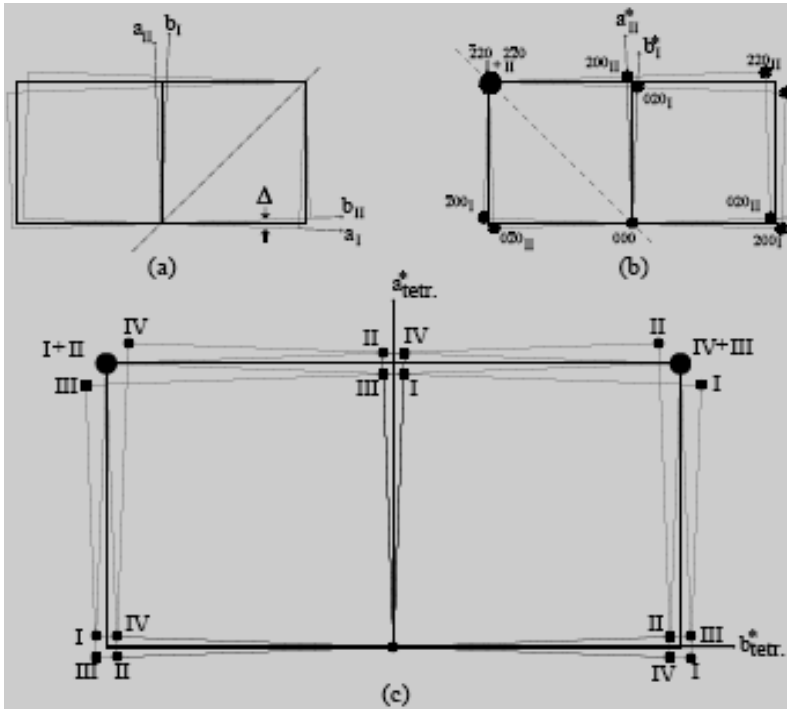


Fig. 8

- (a) orthorhombic distortion with twinning correspondent to a (1-10) mirroring
- (b) corresponding reciprocal lattice
- (c) Overlay of (110)- and (1-10)-mirroring in reciprocal space

In the HTT phase only reflections with h, k, l of equal parity (g for even, u for uneven) are allowed - (uuu) and (ggg). They are called in the following main structure reflections.

In the LTO phase additional reflections occur, called super structure reflections: In the $Abma$ -Structure (ugg), $l \neq 0$ and (guu), in the $Bmab$ structure (gug), $l \neq 0$ and (ugu).

Forbidden in both the HTT and the LTO phase are (uug), (ggu), ($ug0$) and ($gu0$).

These extinction rules will become important later.

In the real structure of the crystal there exist four domain types in total. They are separated into two pairs with the couple $Abma_1/Bmab_1$ (I/II) with the (1-10) mirror plane as grain boundary and the couple $Abma_2/Bmab_2$ (III/IV) with the (110) mirror plane as grain boundary (fig. 8).

The following overlaps of reflections result from this twinning:

- No splitting of the (00l) reflections,
- triple splitting of the (hh0) reflections
- fourfold splitting of the (h00) reflections.

An equal distribution of the volumetric portion of each single domain yields a ratio of intensities of 1:2:1 for the triple splitting. The distance $\Delta\omega$ between the centre and the side

peaks of a (hkl) reflex gives because of $(a+b)/2 = a_{1/2}$ an information about the orthorhombic a/b splitting. For the triple splitting of a $(hh0)$ reflex is valid:

$$\Delta\omega = 90^\circ - 2\arctan(b/a)$$

Thus, although the real crystal is twinned, one can quantify the orthorhombic distortion.

The intensity contribution of the single domains corresponding to the whole intensity of a reflection can be described (taking into account the incoherent overlap of single intensities and the volumetric portions V_{A1} to V_{B2} of the domains) as follows:

$$\begin{aligned} I_{\text{obs}}(hkl) &= I_{Abma1}(hkl) + I_{Bmab1}(hkl) + I_{Abma2}(hkl) + I_{Bmab2}(hkl) \text{ or} \\ V_{\text{total}}|F_{\text{obs}}(hkl)|^2 &= V_{A1}|F_{Abma1}(hkl)|^2 + V_{B1}|F_{Bmab1}(hkl)|^2 + V_{A2}|F_{Abma2}(hkl)|^2 + V_{B2}|F_{Bmab2}(hkl)|^2 \\ &= (V_{A1} + V_{A2})|F_{Abma1}(hkl)|^2 + (V_{B1} + V_{B2})|F_{Bmab1}(hkl)|^2 \\ &= V_{\text{total}} \{ \alpha |F_{Abma}(hkl)|^2 + (1-\alpha) |F_{Abma}(hkl)|^2 \} \end{aligned}$$

with α being the relative portion of the volume of *Abma* domains to the crystal..

Because of the extinction rules in the LTO phase for the super structure reflections is valid: $I_{\text{obs}}(hkl) \sim \alpha |F_{Abma}(hkl)|^2$ for *Abma* and $I_{\text{obs}}(hkl) \sim (1-\alpha) |F_{Abma}(hkl)|^2$ for *Bmab*. Thus, one can classify directly intensities to the volumetric portions of the domain types *Abma* and *Bmab* respectively. Therefore, by using one single additional parameter α to describe the relation between the twins in the structure one can determine the orthorhombic single crystal structure! This holds true although the Bragg reflections contain contributions of up to four different domains.

4.3 Oxygen Position

The oxygen atoms undergo the largest shift of their positions during the transition to the LTO phase. For the structure factor of a any Bragg reflection forbidden in $F4/mmm$ is valid:

$$F(hkl) \sim \sum_i s_i \exp(-2\pi i(hx_i + ky_i + lz_i)) = F(hkl)_{\text{apex oxygen}} + F(hkl)_{\text{in plane oxygen}} + F(hkl)_{\text{structure w/o O}} \\ \rightarrow F(hkl)_{\text{apex oxygen}} + F(hkl)_{\text{in plane oxygen}}$$

In the LTO phase the atomic position of the apex oxygens is (x 0 z), the atomic position for the in-plane oxygens is (1/4 1/4 -z). This yields the following intensities for the superstructure reflections:

$$F(hkl)_{\text{apex oxygen}} = \cos(2\pi hx)\cos(2\pi lz) \text{ for } h \text{ even or} \\ F(hkl)_{\text{apex oxygen}} = \sin(2\pi hx)\cos(2\pi lz) \text{ for } h \text{ uneven}$$

In the case of x-rays the form factor $f_i \sim Z_i$, Z_i =order number is much smaller for oxygen ($Z=16$) than for Cu ($Z=29$) and La ($Z=57$). Because of $I_{\text{obs}}(hkl) \sim |F(hkl)|^2$ the oxygen shift is hardly measurable. In the case of neutrons the scattering lengths b_i of all atoms are in the same order of magnitude ($b_{\text{O}}=5.803$ barn, $b_{\text{Cu}}=$ barn, $b_{\text{La}}=$ barn, 1 barn = 10^{-24} cm²). Therefore, the intensity contribution of the oxygen atoms increases in relation to the other elements in the structure and allows a much more precise determination of the structural change of the oxygen positions

5 Preparatory Exercises

1. What is the fundamental difference between powder/single crystal diffraction and what are the advantages and disadvantages of both techniques (Compare d-values and orientations of different reflections in a cubic structure)?
2. What is wrong with fig. 2?
3. Which reflections are not allowed in a face centered structure (structure factor)?
4. There is no space group $F4/mmm$ in the international tables. Why (Which other space group in the international tables yields the same pattern in direct space)?

6 Experiment Procedure

During this practical course not all physical and technical aspects of structure analysis with neutrons can be discussed in detail. Nevertheless this course is supposed point out the basic similarities and dissimilarities of x-rays and neutron radiation as well as their specific advantages and disadvantages in general and referring to single crystal diffraction. The sample selected for this practical course is most suitable for this purpose because of its special crystallographic peculiarities.

6.1 The Instrument

Fig. 5 shows the typical setup of a single crystal diffractometer with a single detector. Outgoing from the radiation source a primary beam defined by primary optics (in our case the beam tube) reaches the single crystal sample. If one lattice plane (hkl) fulfills Braggs laws, the scattered beam, called secondary beam, leaves the sample under an angle 2Θ to the primary beam. The exact direction of this beam depends only on the relative orientation of the sample to the primary beam.

For the diffractometer shown in fig. 5 the movement of the neutron detector is limited to a horizontal rotation around the 2Θ axis. Thus, only those reflections can be measured, whose scattering vector \mathbf{Q} lies exactly in the plane defined by the source, the sample and detector circle. This plane is also called scattering plane.

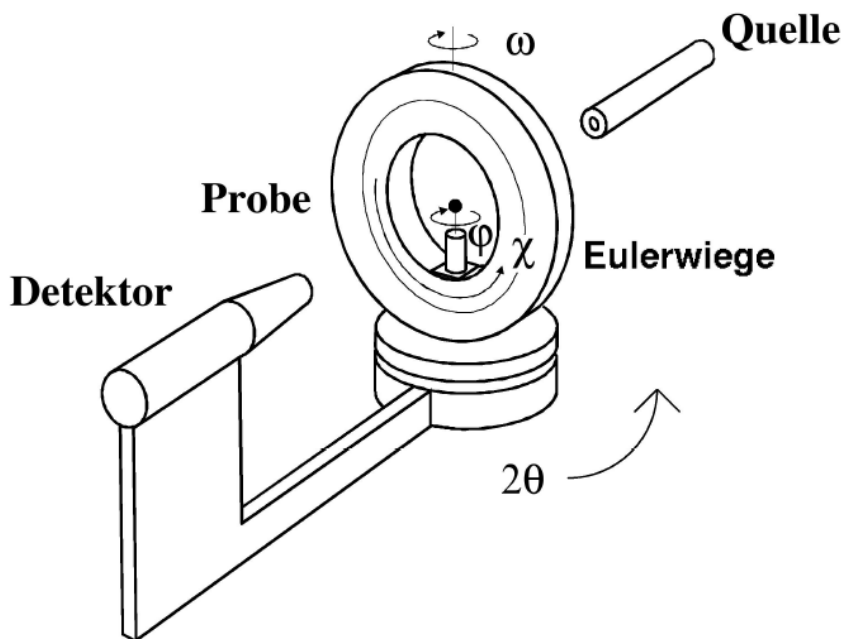


Fig. 5: Scheme of a single crystal diffractometer

To direct the secondary beam towards the detector position one has to orient the sample around the three axes ω , χ and ϕ . These three axes allow a virtually random orientation of the crystal in the primary beam. During the experiment the sample has to stay exactly in the cross point of all four axes (2Θ , ω , χ and ϕ) and the primary beam. Additionally, for $2\Theta = \omega = \chi = \phi = 0^\circ$ the primary beam direction and the χ axis on one hand side and the 2Θ -, ω - and ϕ -axes on the other hand side are identical while the angle between the primary beam and the 2Θ -is exactly 90° . Because of the four rotational axes (2Θ , ω , χ , ϕ) this kind of single crystal diffractometer is often called four circle diffractometer. Another often used geometry - the so called κ -Geometrie - will not be discussed in detail here.

Further details of the experimental setup:

1. Beam source and primary optics: The primary beam is generated by a suitable source (x-rays: x-ray tube, synchrotron; neutrons: nuclear fission, spallation source). The primary optics defines the path of the beam to the sample in the Eulerian cradle. Furthermore, the primary optics defines the beam diameter using slits to make it fit to the sample size for homogeneous illumination. This homogeneity is very important because the quality of the data refinement relies on the comparison of the intensity ratios between the different reflections measured during an experiment. Wrong ratios caused by inhomogeneous illumination can yield wrong structural details! Other components of the primary optics are collimators defining beam divergence and filters or monochromators which define the wavelength λ of the radiation.

2. Sample and sample environment: The sample position is fixed by the centre of the Eulerian cradle which is defined by the cross point of the axes ω , χ and ϕ . As described above, the cradle itself has in combination with the ω -circle the task to orient the sample according to the observed reflection in a way that it hits the detector. The sample itself is mounted on a goniometer head. This head allows the adjustment of the sample in all three directions **x**; **y**; **z**, via microscope or camera. To avoid scattering from the sample environment and goniometer head the sample is usually connected to the head via a thin glass fibre (x-rays) or aluminum pin (neutrons). This reduces significantly background scattering. For experiments at high or low temperatures adjustable cooling or heating devices can be mounted into the Eulerian cradle.

3. Secondary optics and detector: The 2Θ arm of the instrument hold the detector which – in the ideal case – catches only radiation scattered from the sample and transforms it to an electrical signal. There exists a variety of detectors, single detectors and position sensitive 1D and 2D detectors. Area detectors have a large sensitive area that allows the accurate observation of spatial distribution of radiation. Other components of the secondary optics are slits and collimators or analyser (as optional units). They fulfil the task to shield the detector from unwanted radiation like scattering from sample environment, scattering in air, wrong wavelengths or fluorescence

6.2 Sequence of measurement in Theory

1. Centering: In advance of the planned scientific program (profile analysis, Bragg data collection) the orientation of the sample in relation to the coordinate system of the diffractometer has to be determined. First of all the sample has to be centered optically to assure a homogeneous illumination of the sample. Afterwards, a reflection search routine has to be started to optimize the intensity of a found reflection by moving several angles after each other.

In many cases there are some structural informations like the unit cell and hkl values of strong reflections available from previous studies, e.g. from powder diffraction, thus, one can limit the reflection search to 2Θ values around these strong reflections to spare some time and to classify manually the found reflections with the correct indices.

2. Determination of orienting matrix and lattice constants: The comparison of the \mathbf{Q} vectors of the found and centered reflections yields generally one or more suggestions for a suitable unit cell. This is done by a least squares routine minimizing the error bars between the calculated and measured \mathbf{Q} vectors. This method allows to determine accurately the orientation matrix $\mathbf{M}_0 = (\mathbf{a}^* \ \mathbf{b}^* \ \mathbf{c}^*)^T$ of the sample relative to the coordinate system of the diffractometer and the lattice constants of the unit cell.

On HEiDi the axes are defined as following: \mathbf{x} =primary beam, $\mathbf{z} \parallel 2\Theta$ axis, $\mathbf{y}=\mathbf{z} \times \mathbf{x}$.

A proposed unit cell is only acceptable if all experimentally found reflections can be indexed with integer hkl , this means $\mathbf{Q} = (h \ k \ l) * \mathbf{M}_0$. In addition the found reflection intensities I offer a course check, e.g. whether extinction rules are followed or intensities of symmetrically identical reflections are identical.

3. Profile analyses and scan types: During profile analysis reflex profiles are analysed via so called ω scans. During this scan the sample is turned for n steps around a center position ω_0 . This scan makes different crystallites in one large sample visible. In addition one has to take into account that even in perfectly grown crystals there are grain boundaries and slight mismatches of the crystallites. These mosaic blocks are perfect crystals whose orientations are misaligned only a few tenths of a degree or less. By the way, the axis position $2\Theta/2=\Theta=\omega$ is called the bisecting orientation of the Eulerian cradle.

As long as the vertical aperture is large enough, a rotation of the crystal around a ω_0 , that is equivalent to the ideal Θ_0 Bragg angle of a reflex allows to catch the intensity portion of each crystallite in the sample in the neutron detector on the fixed 2Θ position, even those that can only be found for slightly differing ω . Therefore, a crystal with large mosaicity gives measurable intensities over a broader ω area than a perfect crystal. Thus it gives a broader reflex profile. Also the tearing and cracking of a crystal creates broad but unregular profiles. Beside the crystal quality also the instrumental resolution limits the measurable profile widths in the following sense: The divergence of a primary beam in real experiment is limited, for instance to 0.2° .

If a reflection fulfills Bragg's Law at Θ , the total divergence is a convolution of the divergence of the primary beam *and* the mosaicity/divergence of the sample. Thus, the reflection profile will never be sharper than the divergence of the primary beam itself.

In addition one has to take into account that for larger diffraction angles a fixed detector window will not be sufficient to catch the whole reflection intensities during a rocking scan.

For a given spectrum $\Delta\lambda/\lambda$ of the primary beam, with increasing scattering angle Θ angular range $\Delta\Theta$ increases with $\sin(\Delta\Theta/2) = \tan(\Theta) * \Delta\lambda/\lambda$ for which all wavelengths in the interval $\lambda \pm \Delta\lambda/2$ fulfilling Bragg's law are distributed. Because of the limited width of the detector window this yields a cut off of intensities for larger scattering angles for ω -scans.

To compensate this cut off effect it is necessary to begin at a certain 2Θ -angle to move the detector window with the ω -angle.. This can be done by so called $\omega/2\Theta$ -scans. The start position of this 2Θ range depends on the primary beam divergence and sample quality and has to be checked individually for each sample.

4. Collection of Bragg reflections: If a sample was found good after the described preliminary studies one can start with the Bragg data collection. In this data collection all (or selected) reflections in a given 2Θ intervall are collected automatically. The usual strategy follows the rule „Only as many as necessary“. This means the following: On one hand side the quality of the measured reflections has to fulfil certain standards (like small standard deviations σ and a good shape of the profiles) to reach an acceptable accuracy. On the other side there is only a limited amount of time available for each reflection due to the huge number of them (up to several thousands). and the limited beam time. A rule of thumb is therefore to measure about 10 non symmetry equivalent reflections for each free parameter used in the data refinement to get the correct structure. To achieve this goal a typical algorithm is to do a prescan with t_{\min} per point of measurement in combination with a given larger (e.g. $I/\sigma=4$ and 25%, respectively) and a smaller (e.g. $I/\sigma=20$ and 5%, respectively) relative error limit. t_{\min} is chosen in a way that the statistics of strong reflections is fine already after the prescan. Weak reflections are also noticed in the prescan and stored as weak reflections without additional treatment. Reflections in between get an additional chance to improve their statistics by performing a second scan with a limited amount of time up to $t_{\max}-t_{\min}$. This method avoids to spend unreasonable beam time to weak reflections which will not help to improve the quality of the structure model.

6.3 and in Practice

- 1. Adjust optically the sample in the neutron beam :** Alignment of the sample in the rotational centre of the instrument. This is necessary for a homogeneous illumination of the sample for all possible orientations.
- 2. Search for Bragg reflections and center them, , “Reflex centering”:** Sample and detector position are controlled by a special diffractometer software. The main goal is to find suitable angular positions for the detector first and afterwards for the sample to get a measurable signal. Afterwards the orientation of the sample in the Eulerian cradle have to be optimized for maximum intensity.
- 3. Analyse profiles of selected reflections:** Study different reflex profiles and reveal the impact of twinning
- 4. Determine the orthorhombic lattice parameters a, b and c:** Estimate the misalignment of a and b in reference to $a_{1/2}$ in the real tetragonal cell.

5. **Determine the average tetragonal unit cell:** The centering of different reflections allows the calculation of all lattice constants including the averaged tetragonal parameters.
6. **Observe super structure reflections:** Measuring pairs of $(hkl)/(khl)$ allows the estimation of the volumetric contribution of each single domain to the whole crystal.
7. **Select measurement parameters for Bragg data collection:** In order to optimize the number and statistical quality of collected Bragg reflections suitable scan parameters (time/step, no. of steps, stepwidths, etc.) have to be determined.
8. **Collect a Bragg data set**

6.4 Data analysis

After having measured a Bragg data set one has to do the final step, the alignment of model and measurement:

1. **Data Reduction:** In this process the measured reflection profiles are analysed and reduced to a simple list of all measured reflections and their integrated intensities including error bars and some other useful information. This so-called hkl -list is the base for the next step:
2. **Structure refinement:** Here the measured hkl -list and our structure model are combined to determine structural details like atomic positions and mean square displacements.

7 Experiment-Related Exercises

1. Why is the optical adjustment of the sample so important?
2. How large is the a/b -splitting at room temperature ($=|a-b|/(a+b)$)?
3. What is the benefit/enhancement of studying the room temperature structure with neutrons instead of X-rays?

References

- [1] Th. Hahn (ed.), Space-group symmetry, International Tables for Crystallography Vol. A, Kluver Academic Publishers (2006).
- [2] W.H. Zachariasen, *Acta Cryst.* 18 703 (1965).
- [3] W.H. Zachariasen, *Acta Cryst.* 18 705 (1965).
- [4] P. Coppens and W.C. Hamilton, *Acta Cryst. A* 26 71-83 (1970).
- [5] P.J. Becker and P. Coppens, *Acta Cryst. A* 30 129-147 (1974).
- [6] P.J. Becker and P. Coppens, *Acta Cryst. A* 30 148-153 (1974).
- [7] U.H. Zucker, E. Perrenthaler, W.F. Kuhs, R. Bachmann and H. Schulz *J. of Appl. Crystallogr.*, 16 358 (1983).
- [8] P. Coppens, W.C. Hamilton, S. Wilkins, M.S. Lehmann and Savariault, *Datap*, http://www.ill.fr/data_treat/diftreat.html#single (1999).
- [9] J. Bednorz and K. Müller, *Z. Phys. B* 64 189 (1986).

Literature

- N.W. Ashcroft and N.D. Mermin, *Festkörperphysik*, Oldenbourg 2001.
- H. Ibach and H. Lüth, *Festkörperphysik, Einführung in die Grundlagen*, 6. Edition Springer 2002.
- C. Kittel, *Einführung in die Festkörperphysik*, 10. Edition, Oldenbourg 1993.
- W. Borchardt-Ott, *Kristallographie. Eine Einführung für Naturwissenschaftler*, 6. Auflage Springer 2002.
- W. Kleber, *Einführung in die Kristallographie*, Oldenbourg 1998
- H. Dachs, *Neutron Diffraction*, Springer (1978)
- D.J. Dyson, *X-Ray and Electron Diffraction Studies in Material Science*, Maney Pub 2004.
- C. Giacovazzo, *Fundamentals of Crystallography*, 2nd Ed., Oxford University Press 2002.
- L.A. Aslanov, *Crystallographic Instrumentation*, Oxford University Press 1998.
- M.T. Dove, *Structure and Dynamics. An Atomic View of Materials*, Oxford University Press 2003.
- W. Clegg, *Crystal Structure Analysis. Principles and Practice*, Oxford University Press 2001.

Appendix (Tables and space groups from [1])

3.1. SPACE-GROUP DETERMINATION AND DIFFRACTION SYMBOLS

Table 3.1.4.1. *Reflection conditions, diffraction symbols and possible space groups (cont.)*

ORTHORHOMBIC, Laue class mmm ($2/m\ 2/m\ 2/m$) (cont.)

Reflection conditions								Laue class mmm ($2/m\ 2/m\ 2/m$)		
hkl	$0kl$	$h0l$	$hk0$	$h00$	$0k0$	$00l$	Extinction symbol	Point group		
								222	$mm2$ $m2m$ $2mm$	mmm
$h+k$	$k+l$	l	k		k	l	$Pncb$	C222 (21)	Pnn2 (34)	$Pncb$ (50)
	$k+l$	l	$h+k$	h	k	l	$Pncn$			$Pncn$ (52)
	$k+l$	$h+l$		h	k	l	$Pnn-$			Pnnm (58)
	$k+l$	$h+l$	h	h	k	l	$Pnna$			Pnna (52)
	$k+l$	$h+l$	k	h	k	l	$Pnnb$			$Pnnb$ (52)
	$k+l$	$h+l$	$h+k$	h	k	l	$Pnnn$			Pnnn (48)
	k	h	$h+k$	h	k		$C----$			Cmmm (65)
$h+k$	k	h	$h+k$	h	k	l	$C-2_1$	C222₁ (20)	Cmm2 (35) $Cm2m$ (38) $C2mm$ (38)	
$h+k$	k	h	h, k	h	k		$C-(ab)$			$Cm2e$ (39)
										$C2me$ (39)
$h+k$	k	h, l	$h+k$	h	k	l	$C-c-$			Cmc2₁ (36)
										$C2cm$ (40)
$h+k$	k	h, l	h, k	h	k	l	$C-c(ab)$			$C2ce$ (41)
$h+k$	k, l	h	$h+k$	h	k	l	$Cc--$			$Ccm2_1$ (36)
										$Cc2m$ (40)
$h+k$	k, l	h	h, k	h	k	l	$Cc-(ab)$	B222 (21)	Bmm2 (38) $Bm2m$ (35) $B2mm$ (38)	$Cc2e$ (41)
$h+k$	k, l	h, l	$h+k$	h	k	l	$Ccc-$			Cce2 (37)
$h+k$	k, l	h, l	h, k	h	k	l	$Ccc(ab)$			$Ccme$ (64)
$h+l$	l	$h+l$	h	h		l	$B----$			Ccem (66)
										Ccee (68)
										$Bmmn$ (65)
$h+l$	l	$h+l$	h, k	h	k	l	$B-2_1-$			
$h+l$	l	$h+l$		h	k	l	$B--b$			$Bm2_1b$ (36)
								B22₁2 (20)	$B2mb$ (40) $Bme2$ (39) $B2em$ (39)	$Bmbm$ (63)
$h+l$	l	h, l	h	h		l	$B-(ac)-$			$Bmem$ (67)
$h+l$	l	h, l	h, k	h	k	l	$B-(ac)b$			$B2eb$ (41)
										$Bmeb$ (64)
$h+l$	k, l	$h+l$	h	h	k	l	$Bb--$			$Bbm2$ (40)
										$Bb2_1m$ (36)
$h+l$	k, l	$h+l$	h, k	h	k	l	$Bb-b$			$Bb2b$ (37)
$h+l$	k, l	h, l	h	h	k	l	$Bb(ac)-$	A222 (21)	Amm2 (38) $Am2m$ (38) $A2mm$ (35)	$Bbmb$ (66)
$h+l$	k, l	h, l	h, k	h	k	l	$Bb(ac)b$			$Bbem$ (64)
$k+l$	$k+l$	l	k		k	l	$A----$			$Bbeb$ (68)
										$Ammm$ (65)
$k+l$	$k+l$	l	k	h	k	l	$A2_1--$	A2₁22 (20)	Am2a (40) $A2_1ma$ (36) Ama2 (40) $A2_1am$ (36) $A2aa$ (37) Aem2 (39) $Ae2m$ (39)	
$k+l$	$k+l$	l	h, k	h	k	l	$A--a$			$Aema$ (64)
										$Aeam$ (64)
$k+l$	$k+l$	h, l	k	h	k	l	$A-a-$			$Aeaa$ (68)
										Immm (71)
$k+l$	$k+l$	h, l	h, k	h	k	l	$A-aa$			
$k+l$	k, l	l	k		k	l	$A(bc)--$			
$k+l$	k, l	l	h, k	h	k	l	$A(bc)-a$	[I222 (23)]* [I2₁2₁2₁ (24)]*	Aea2 (41) Imm2 (44) $Im2m$ (44)	
$k+l$	k, l	h, l	k	h	k	l	$A(bc)a-$			
$k+l$	k, l	h, l	h, k	h	k	l	$A(bc)aa$			
$h+k+l$	$k+l$	$h+l$	$h+k$	h	k	l	$I----$			

3. DETERMINATION OF SPACE GROUPS

Table 3.1.4.1. *Reflection conditions, diffraction symbols and possible space groups (cont.)*ORTHORHOMBIC, Laue class mmm ($2/m\ 2/m\ 2/m$) (cont.)

Reflection conditions								Laue class mmm ($2/m\ 2/m\ 2/m$)		
hkl	$0kl$	$h0l$	$hk0$	$h00$	$0k0$	$00l$	Extinction symbol	Point group		
								222	$mm2$ $m2m$ $2mm$	mmm
$h+k+l$	$k+l$	$h+l$	h, k	h	k	l	$I - (ab)$		$I2mm$ (44) $Im2a$ (46) $I2mb$ (46) $Ima2$ (46) $I2cm$ (46) $I2cb$ (45) $Iem2$ (46) $Ic2m$ (46)	$Imma$ (74) $Immb$ (74) $Imam$ (74) $Imcm$ (74) $Imcb$ (72) $Iemm$ (74)
$h+k+l$	$k+l$	h, l	$h+k$	h	k	l	$I - (ac) -$			
$h+k+l$	$k+l$	h, l	h, k	h	k	l	$I - cb$			
$h+k+l$	k, l	$h+l$	$h+k$	h	k	l	$I(bc) - -$			
$h+k+l$	k, l	$h+l$	h, k	h	k	l	$Ic - a$		$Ic2a$ (45)	$Icma$ (72)
$h+k+l$	k, l	h, l	$h+k$	h	k	l	$Iba -$		$Iba2$ (45)	$Ibam$ (72)
$h+k+l$	k, l	h, l	h, k	h	k	l	$Ibca$			$Ibca$ (73) $Icab$ (73)
$h+k, h+l, k+l$	k, l	h, l	h, k	h	k	l	$F - - -$	$F222$ (22)	$Fmm2$ (42) $Fm2m$ (42) $F2mm$ (42) $F2dd$ (43) $Fd2d$ (43) $Fdd2$ (43)	$Fmmm$ (69)
$h+k, h+l, k+l$	k, l	$h+l = 4n; h, l$	$h+k = 4n; h, k$	$h = 4n$	$k = 4n$	$l = 4n$	$F-dd$			
$h+k, h+l, k+l$	$k+l = 4n; k, l$	h, l	$h+k = 4n; h, k$	$h = 4n$	$k = 4n$	$l = 4n$	$Fd-d$			
$h+k, h+l, k+l$	$k+l = 4n; k, l$	$h+l = 4n; h, l$	h, k	$h = 4n$	$k = 4n$	$l = 4n$	$Fdd-$			
$h+k, h+l, k+l$	$k+l = 4n; k, l$	$h+l = 4n; h, l$	$h+k = 4n; h, k$	$h = 4n$	$k = 4n$	$l = 4n$	$Fddd$			$Fddd$ (70)

* Pair of space groups with common point group and symmetry elements but differing in the relative location of these elements.

3.1. SPACE-GROUP DETERMINATION AND DIFFRACTION SYMBOLS

Table 3.1.4.1. *Reflection conditions, diffraction symbols and possible space groups (cont.)*TETRAGONAL, Laue classes $4/m$ and $4/mmm$ (cont.)

								Laue class						
Reflection conditions								4/m			4/mmm (4/m 2/m 2/m)			
								Point group						
hkl	hk0	0kl	hhl	00l	0k0	h0h	Extinction symbol	4	$\bar{4}$	4/m	422	4mm	$\bar{4}2m$ $\bar{4}m2$	4/mmm
	h + k	k					k	Pnb –						P4/nbm (125)
	h + k	k	l	l	k			Pnbc						P4 ₂ /nbc (133)
	h + k	l		l	k			Pnc –						P4 ₂ /ncm (138)
	h + k	l	l	l	k			Pncc						P4/ncc (130)
	h + k	k + l		l	k			Pnn –						P4 ₂ /nmm (134)
	h + k	k + l	l	l	k			Pnnc						P4/nnc (126)
h + k + l	h + k	k + l	l	l	k		l – – –	I4 (79)	I $\bar{4}$ (82)	I4/m (87)	I422 (97)	I4mm (107)	I $\bar{4}2m$ (121)	I4/mmm (139)
													I $\bar{4}m2$ (119)	
h + k + l	h + k	k + l	l	l = 4n	k		I4 ₁ – –	I4 ₁ (80)			I4 ₁ 22 (98)			
h + k + l	h + k	k + l	$\frac{\ddagger}{2}$	l = 4n	k	h	l – – d					I4 ₁ md (109)	I $\bar{4}2d$ (122)	
h + k + l	h + k	k, l	l	l	k		l – c –					I4cm (108)	I $\bar{4}c2$ (120)	I4/mcm (140)
h + k + l	h + k	k, l	$\frac{\ddagger}{2}$	l = 4n	k	h	l – cd					I4 ₁ cd (110)		
h + k + l	h, k	k + l	l	l = 4n	k		I4 ₁ /a – –			I4 ₁ /a (88)				
h + k + l	h, k	k + l	$\frac{\ddagger}{2}$	l = 4n	k	h	la – d							I4 ₁ /amd (141)
h + k + l	h, k	k, l	$\frac{\ddagger}{2}$	l = 4n	k	h	lacd							I4 ₁ /acd (142)

† Pair of enantiomorphic space groups, cf. Section 3.1.5.

‡ Condition: $2h+l = 4n; l$.

International Tables for Crystallography (2006). Vol. A, Space group 139, pp. 478–479.

$I4/mmm$

D_{4h}^{17}



$4/mmm$

Tetragonal

No. 139

$I\ 4/m\ 2/m\ 2/m$

Patterson symmetry $I4/mmm$

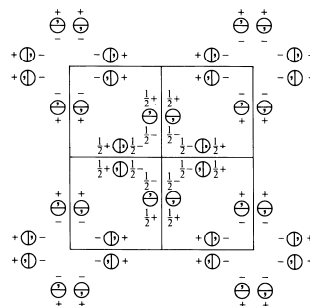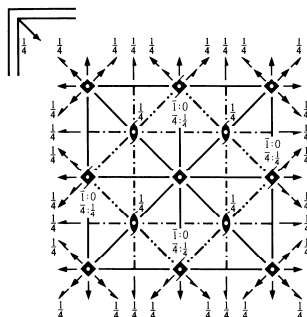

Origin at centre ($4/mmm$)

Asymmetric unit $0 \leq x \leq \frac{1}{2}; 0 \leq y \leq \frac{1}{2}; 0 \leq z \leq \frac{1}{2}; x \leq y$

Symmetry operations

For $(0, 0, 0) + \text{set}$

- | | | | |
|-------------------------|--------------------|-------------------------------|-------------------------------|
| (1) 1 | (2) 2 $0, 0, z$ | (3) 4^+ $0, 0, z$ | (4) 4^- $0, 0, z$ |
| (5) 2 $0, y, 0$ | (6) 2 $x, x, 0$ | (7) 2 $x, x, 0$ | (8) 2 $x, \bar{x}, 0$ |
| (9) $\bar{1}$ $0, 0, 0$ | (10) m $x, y, 0$ | (11) 4^+ $0, 0, z; 0, 0, 0$ | (12) 4^- $0, 0, z; 0, 0, 0$ |
| (13) m $x, 0, z$ | (14) m $0, y, z$ | (15) m x, \bar{x}, z | (16) m x, x, z |

For $(\frac{1}{2}, \frac{1}{2}, \frac{1}{2}) + \text{set}$

- | | | | |
|-----------------------------------------------------------|-----------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|
| (1) $r(\frac{1}{2}, \frac{1}{2}, \frac{1}{2})$ | (2) $2(0, 0, \frac{1}{2})$ $\frac{1}{2}, \frac{1}{2}, z$ | (3) $4^+(0, 0, \frac{1}{2})$ $0, \frac{1}{2}, z$ | (4) $4^-(0, 0, \frac{1}{2})$ $\frac{1}{2}, 0, z$ |
| (5) $2(0, \frac{1}{2}, 0)$ $\frac{1}{2}, y, \frac{1}{2}$ | (6) $2(\frac{1}{2}, 0, 0)$ $x, \frac{1}{2}, \frac{1}{2}$ | (7) $2(\frac{1}{2}, \frac{1}{2}, 0)$ $x, x, \frac{1}{2}$ | (8) 2 $x, \bar{x} + \frac{1}{2}, \frac{1}{2}$ |
| (9) $\bar{1}$ $\frac{1}{2}, \frac{1}{2}, \frac{1}{2}$ | (10) $n(\frac{1}{2}, \frac{1}{2}, 0)$ $x, y, \frac{1}{2}$ | (11) 4^+ $\frac{1}{2}, 0, z; \frac{1}{2}, 0, \frac{1}{2}$ | (12) 4^- $0, \frac{1}{2}, z; 0, \frac{1}{2}, \frac{1}{2}$ |
| (13) $n(\frac{1}{2}, 0, \frac{1}{2})$ $x, \frac{1}{2}, z$ | (14) $n(0, \frac{1}{2}, \frac{1}{2})$ $\frac{1}{2}, y, z$ | (15) c $x \mid \frac{1}{2}, \bar{x}, z$ | (16) $n(\frac{1}{2}, \frac{1}{2}, \frac{1}{2})$ x, x, z |

Maximal non-isomorphic subgroups (continued)

- IIa**
- | | |
|----------------------|-----------------------------------------------------------------------------------------------------|
| [2] $P4_2/nmc$ (137) | 1; 2; 7; 8; 11; 12; 13; 14; (3; 4; 5; 6; 9; 10; 15; 16) + $(\frac{1}{2}, \frac{1}{2}, \frac{1}{2})$ |
| [2] $P4_2/mnm$ (136) | 1; 2; 7; 8; 9; 10; 15; 16; (3; 4; 5; 6; 11; 12; 13; 14) + $(\frac{1}{2}, \frac{1}{2}, \frac{1}{2})$ |
| [2] $P4_2/nmm$ (134) | 1; 2; 5; 6; 11; 12; 15; 16; (3; 4; 7; 8; 9; 10; 13; 14) + $(\frac{1}{2}, \frac{1}{2}, \frac{1}{2})$ |
| [2] $P4_2/mmc$ (131) | 1; 2; 5; 6; 9; 10; 13; 14; (3; 4; 7; 8; 11; 12; 15; 16) + $(\frac{1}{2}, \frac{1}{2}, \frac{1}{2})$ |
| [2] $P4_2/nmm$ (129) | 1; 2; 3; 4; 13; 14; 15; 16; (5; 6; 7; 8; 9; 10; 11; 12) + $(\frac{1}{2}, \frac{1}{2}, \frac{1}{2})$ |
| [2] $P4/mnc$ (128) | 1; 2; 3; 4; 9; 10; 11; 12; (5; 6; 7; 8; 13; 14; 15; 16) + $(\frac{1}{2}, \frac{1}{2}, \frac{1}{2})$ |
| [2] $P4/nnc$ (126) | 1; 2; 3; 4; 5; 6; 7; 8; (9; 10; 11; 12; 13; 14; 15; 16) + $(\frac{1}{2}, \frac{1}{2}, \frac{1}{2})$ |
| [2] $P4/mmm$ (123) | 1; 2; 3; 4; 5; 6; 7; 8; 9; 10; 11; 12; 13; 14; 15; 16 |

IIb none

Maximal isomorphic subgroups of lowest index

IIc [3] $I4/mmm$ ($c' = 3c$) (139); [9] $I4/mmm$ ($a' = 3a, b' = 3b$) (139)

Minimal non-isomorphic supergroups

I [3] $Fm\bar{3}m$ (225); [3] $Im\bar{3}m$ (229)

II [2] $C4/mmm$ ($c' = \frac{1}{2}c$) ($P4/mmm$, 123)

Copyright © 2006 International Union of Crystallography

CONTINUED

No. 139

 $I4/mmm$ **Generators selected** (1); $t(1,0,0)$; $t(0,1,0)$; $t(0,0,1)$; $t(\frac{1}{2}, \frac{1}{2}, \frac{1}{2})$; (2); (3); (5); (9)**Positions**Multiplicity,
Wyckoff letter,
Site symmetryCoordinates
(0,0,0)+ $(\frac{1}{2}, \frac{1}{2}, \frac{1}{2})$ +

Reflection conditions

General:

32	<i>o</i>	1	(1) x, y, z	(2) \bar{x}, \bar{y}, z	(3) \bar{y}, x, z	(4) y, \bar{x}, z
			(5) \bar{x}, y, \bar{z}	(6) x, \bar{y}, \bar{z}	(7) y, x, \bar{z}	(8) $\bar{y}, \bar{x}, \bar{z}$
			(9) $\bar{x}, \bar{y}, \bar{z}$	(10) x, y, \bar{z}	(11) y, \bar{x}, \bar{z}	(12) \bar{y}, x, \bar{z}
			(13) x, \bar{y}, z	(14) \bar{x}, y, z	(15) \bar{y}, \bar{x}, z	(16) y, x, z

 $hkl : h+k+l=2n$
 $hk0 : h+k=2n$
 $0kl : k+l=2n$
 $hhl : l=2n$
 $00l : l=2n$
 $h00 : h=2n$

Special: as above, plus

16	<i>n</i>	$.m.$	$0, y, z$ $0, \bar{y}, \bar{z}$	$0, \bar{y}, z$ $0, y, \bar{z}$	$\bar{y}, 0, z$ $y, 0, \bar{z}$	$y, 0, z$ $\bar{y}, 0, \bar{z}$
16	<i>m</i>	$. . m$	x, x, z $\bar{x}, \bar{x}, \bar{z}$	\bar{x}, \bar{x}, z x, x, \bar{z}	\bar{x}, x, z x, \bar{x}, \bar{z}	x, \bar{x}, z $\bar{x}, \bar{x}, \bar{z}$
16	<i>l</i>	$m . .$	$x, y, 0$ $\bar{x}, \bar{y}, 0$	$\bar{x}, \bar{y}, 0$ $x, y, 0$	$\bar{y}, x, 0$ $y, x, 0$	$y, \bar{x}, 0$ $\bar{y}, \bar{x}, 0$
16	<i>k</i>	$. . 2$	$x, x+\frac{1}{2}, \frac{1}{2}$ $\bar{x}, \bar{x}+\frac{1}{2}, \frac{1}{2}$	$\bar{x}, \bar{x}+\frac{1}{2}, \frac{1}{2}$ $x, x+\frac{1}{2}, \frac{1}{2}$	$\bar{x}+\frac{1}{2}, x, \frac{1}{2}$ $x+\frac{1}{2}, \bar{x}, \frac{1}{2}$	$x+\frac{1}{2}, \bar{x}, \frac{1}{2}$ $\bar{x}+\frac{1}{2}, x, \frac{1}{2}$
8	<i>j</i>	$m 2 m .$	$x, \frac{1}{2}, 0$	$\bar{x}, \frac{1}{2}, 0$	$\frac{1}{2}, x, 0$	$\frac{1}{2}, \bar{x}, 0$
8	<i>i</i>	$m 2 m .$	$x, 0, 0$	$\bar{x}, 0, 0$	$0, x, 0$	$0, \bar{x}, 0$
8	<i>h</i>	$m . 2 m$	$x, x, 0$	$\bar{x}, \bar{x}, 0$	$\bar{x}, x, 0$	$x, \bar{x}, 0$
8	<i>g</i>	$2 m m .$	$0, \frac{1}{2}, z$	$\frac{1}{2}, 0, z$	$0, \frac{1}{2}, \bar{z}$	$\frac{1}{2}, 0, \bar{z}$
8	<i>f</i>	$. . 2/m$	$\frac{1}{2}, \frac{1}{2}, \frac{1}{2}$	$\frac{1}{2}, \frac{3}{2}, \frac{1}{2}$	$\frac{3}{2}, \frac{1}{2}, \frac{1}{2}$	$\frac{1}{2}, \frac{3}{2}, \frac{1}{2}$
4	<i>e</i>	$4 m m$	$0, 0, z$	$0, 0, \bar{z}$		
4	<i>d</i>	$\bar{4} m 2$	$0, \frac{1}{2}, \frac{1}{4}$	$\frac{1}{2}, 0, \frac{1}{4}$		
4	<i>c</i>	$m m m .$	$0, \frac{1}{2}, 0$	$\frac{1}{2}, 0, 0$		
2	<i>b</i>	$4/m m m$	$0, 0, \frac{1}{2}$			
2	<i>a</i>	$4/m m m$	$0, 0, 0$			

no extra conditions

no extra conditions

no extra conditions

 $hkl : l=2n$

no extra conditions

no extra conditions

no extra conditions

 $hkl : l=2n$ $hkl : k, l=2n$

no extra conditions

 $hkl : l=2n$ $hkl : l=2n$

no extra conditions

no extra conditions

Symmetry of special projectionsAlong $[001]$ $p4mm$ $\mathbf{a}' = \frac{1}{2}(\mathbf{a} - \mathbf{b})$ $\mathbf{b}' = \frac{1}{2}(\mathbf{a} + \mathbf{b})$ Origin at $0, 0, z$ Along $[100]$ $c2mm$ $\mathbf{a}' = \mathbf{b}$ $\mathbf{b}' = \mathbf{c}$ Origin at $x, 0, 0$ Along $[110]$ $p2mm$ $\mathbf{a}' = \frac{1}{2}(-\mathbf{a} + \mathbf{b})$ $\mathbf{b}' = \frac{1}{2}\mathbf{c}$ Origin at $x, x, 0$ **Maximal non-isomorphic subgroups**

I	[2] $I\bar{4}2m$ (121)	(1; 2; 5; 6; 11; 12; 15; 16)+
	[2] $I\bar{4}m2$ (119)	(1; 2; 7; 8; 11; 12; 13; 14)+
	[2] $I4mm$ (107)	(1; 2; 3; 4; 13; 14; 15; 16)+
	[2] $I422$ (97)	(1; 2; 3; 4; 5; 6; 7; 8)+
	[2] $I4/m11$ ($I4/m$, 87)	(1; 2; 3; 4; 9; 10; 11; 12)+
	[2] $I2/m2/m1$ ($Immm$, 71)	(1; 2; 5; 6; 9; 10; 13; 14)+
	[2] $I2/m12/m$ ($Fmmm$, 69)	(1; 2; 7; 8; 9; 10; 15; 16)+

(Continued on preceding page)

International Tables for Crystallography (2006). Vol. A, Space group 69, pp. 316–318.

Fmm

D_{2h}^{23}


mmm

Orthorhombic

No. 69

$F 2/m 2/m 2/m$

Patterson symmetry Fmm

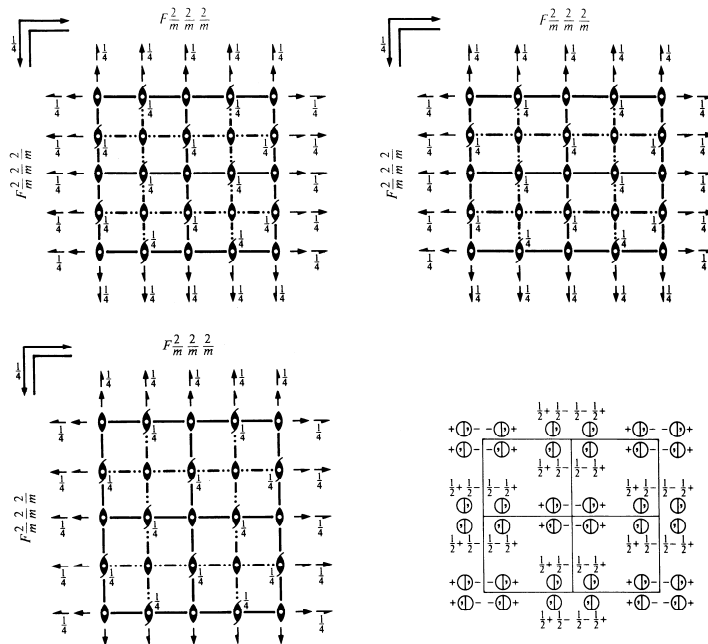

Origin at centre (mmm)

Asymmetric unit $0 \leq x \leq \frac{1}{2}; 0 \leq y \leq \frac{1}{2}; 0 \leq z \leq \frac{1}{2}$

Symmetry operations

For $(0, 0, 0) + \text{set}$

- | | | | |
|-------------------------|-------------------|-------------------|-------------------|
| (1) 1 | (2) $2 \ 0, 0, z$ | (3) $2 \ 0, y, 0$ | (4) $2 \ x, 0, 0$ |
| (5) $\bar{1} \ 0, 0, 0$ | (6) $m \ x, y, 0$ | (7) $m \ x, 0, z$ | (8) $m \ 0, y, z$ |

For $(0, \frac{1}{2}, \frac{1}{2}) + \text{set}$

- | | | | |
|---------------------------------------------|------------------------------------------------|------------------------------------------------|------------------------------------------------|
| (1) $t(0, \frac{1}{2}, \frac{1}{2})$ | (2) $2(0, 0, \frac{1}{2}) \ 0, \frac{1}{2}, z$ | (3) $2(0, \frac{1}{2}, 0) \ 0, y, \frac{1}{2}$ | (4) $2 \ x, \frac{1}{2}, \frac{1}{2}$ |
| (5) $\bar{1} \ 0, \frac{1}{2}, \frac{1}{2}$ | (6) $b \ x, y, \frac{1}{2}$ | (7) $c \ x, \frac{1}{2}, z$ | (8) $n(0, \frac{1}{2}, \frac{1}{2}) \ 0, y, z$ |

For $(\frac{1}{2}, 0, \frac{1}{2}) + \text{set}$

- | | | | |
|---------------------------------------------|------------------------------------------------|------------------------------------------------|------------------------------------------------|
| (1) $t(\frac{1}{2}, 0, \frac{1}{2})$ | (2) $2(0, 0, \frac{1}{2}) \ \frac{1}{2}, 0, z$ | (3) $2 \ \frac{1}{2}, y, \frac{1}{2}$ | (4) $2(\frac{1}{2}, 0, 0) \ x, 0, \frac{1}{2}$ |
| (5) $\bar{1} \ \frac{1}{2}, 0, \frac{1}{2}$ | (6) $a \ x, y, \frac{1}{2}$ | (7) $n(\frac{1}{2}, 0, \frac{1}{2}) \ x, 0, z$ | (8) $c \ \frac{1}{2}, y, z$ |

For $(\frac{1}{2}, \frac{1}{2}, 0) + \text{set}$

- | | | | |
|---------------------------------------------|------------------------------------------------|------------------------------------------------|------------------------------------------------|
| (1) $t(\frac{1}{2}, \frac{1}{2}, 0)$ | (2) $2 \ \frac{1}{2}, \frac{1}{2}, z$ | (3) $2(0, \frac{1}{2}, 0) \ \frac{1}{2}, y, 0$ | (4) $2(\frac{1}{2}, 0, 0) \ x, \frac{1}{2}, 0$ |
| (5) $\bar{1} \ \frac{1}{2}, \frac{1}{2}, 0$ | (6) $n(\frac{1}{2}, \frac{1}{2}, 0) \ x, y, 0$ | (7) $a \ x, \frac{1}{2}, z$ | (8) $b \ \frac{1}{2}, y, z$ |

CONTINUED

No. 69

 Fmm **Generators selected** (1); $t(1,0,0)$; $t(0,1,0)$; $t(0,0,1)$; $t(0,\frac{1}{2},\frac{1}{2})$; $t(\frac{1}{2},0,\frac{1}{2})$; (2); (3); (5)**Positions**Multiplicity,
Wyckoff letter,
Site symmetry

Coordinates

(0,0,0)+ (0, $\frac{1}{2}$, $\frac{1}{2}$)+ ($\frac{1}{2}$,0, $\frac{1}{2}$)+ ($\frac{1}{2}$, $\frac{1}{2}$,0)+

Reflection conditions

General:

32 p 1 (1) x,y,z (2) \bar{x},\bar{y},z (3) \bar{x},y,\bar{z} (4) x,\bar{y},\bar{z}
 (5) \bar{x},\bar{y},\bar{z} (6) x,y,\bar{z} (7) x,\bar{y},z (8) \bar{x},y,z

hkl : $h+k, h+l, k+l = 2n$
 $0kl$: $k, l = 2n$
 $h0l$: $h, l = 2n$
 $hk0$: $h, k = 2n$
 $h00$: $h = 2n$
 $0k0$: $k = 2n$
 $00l$: $l = 2n$

Special: as above, plus

16 o . . m $x,y,0$ $\bar{x},\bar{y},0$ $\bar{x},y,0$ $x,y,0$

no extra conditions

16 n . m . $x,0,z$ $\bar{x},0,\bar{z}$ $\bar{x},0,\bar{z}$ $x,0,\bar{z}$

no extra conditions

16 m m . . $0,y,z$ $0,\bar{y},z$ $0,y,\bar{z}$ $0,\bar{y},\bar{z}$

no extra conditions

16 l 2 . . $x,\frac{1}{4},\frac{1}{4}$ $\bar{x},\frac{3}{4},\frac{1}{4}$ $\bar{x},\frac{3}{4},\frac{3}{4}$ $x,\frac{1}{4},\frac{3}{4}$

 hkl : $h = 2n$

16 k . 2 . $\frac{1}{4},y,\frac{1}{4}$ $\frac{3}{4},\bar{y},\frac{1}{4}$ $\frac{3}{4},\bar{y},\frac{3}{4}$ $\frac{1}{4},y,\frac{3}{4}$

 hkl : $h = 2n$

16 j . . 2 $\frac{1}{4},\frac{1}{4},z$ $\frac{1}{4},\frac{1}{4},\bar{z}$ $\frac{3}{4},\frac{3}{4},\bar{z}$ $\frac{1}{4},\frac{3}{4},z$

 hkl : $h = 2n$

8 i m m 2 $0,0,z$ $0,0,\bar{z}$

no extra conditions

8 h m 2 m $0,y,0$ $0,\bar{y},0$

no extra conditions

8 g 2 m m $x,0,0$ $\bar{x},0,0$

no extra conditions

8 f 2 2 2 $\frac{1}{4},\frac{1}{4},\frac{1}{4}$ $\frac{3}{4},\frac{3}{4},\frac{3}{4}$

 hkl : $h = 2n$

8 e . . 2/ m $\frac{1}{4},\frac{1}{4},0$ $\frac{3}{4},\frac{3}{4},0$

 hkl : $h = 2n$

8 d . 2/ m . $\frac{1}{4},0,\frac{1}{4}$ $\frac{3}{4},0,\frac{1}{4}$

 hkl : $h = 2n$

8 c 2/ m . . $0,\frac{1}{4},\frac{1}{4}$ $0,\frac{3}{4},\frac{1}{4}$

 hkl : $h = 2n$

4 b m m m $0,0,\frac{1}{2}$

no extra conditions

4 a m m m $0,0,0$

no extra conditions

Symmetry of special projections

Along $[001]$ $p2mm$
 $\mathbf{a}' = \frac{1}{2}\mathbf{a}$ $\mathbf{b}' = \frac{1}{2}\mathbf{b}$
 Origin at 0,0, z

Along $[100]$ $p2mm$
 $\mathbf{a}' = \frac{1}{2}\mathbf{b}$ $\mathbf{b}' = \frac{1}{2}\mathbf{c}$
 Origin at $x,0,0$

Along $[010]$ $p2mm$
 $\mathbf{a}' = \frac{1}{2}\mathbf{c}$ $\mathbf{b}' = \frac{1}{2}\mathbf{a}$
 Origin at 0, $y,0$

302

CONTINUED

No. 64

*Cmce***Generators selected** (1); $t(1,0,0)$; $t(0,1,0)$; $t(0,0,1)$; $t(\frac{1}{2}, \frac{1}{2}, 0)$; (2); (3); (5)**Positions**Multiplicity,
Wyckoff letter,
Site symmetry

Coordinates

 $(0,0,0)+$ $(\frac{1}{2}, \frac{1}{2}, 0)+$

Reflection conditions

General:

16	<i>g</i>	1	(1) x, y, z	(2) $\bar{x}, \bar{y} + \frac{1}{2}, z + \frac{1}{2}$	(3) $\bar{x}, y + \frac{1}{2}, \bar{z} + \frac{1}{2}$	(4) x, \bar{y}, \bar{z}
			(5) $\bar{x}, \bar{y}, \bar{z}$	(6) $x, y + \frac{1}{2}, \bar{z} + \frac{1}{2}$	(7) $x, \bar{y} + \frac{1}{2}, z + \frac{1}{2}$	(8) \bar{x}, y, z

 $hkl : h+k=2n$
 $0kl : k=2n$
 $h0l : h, l=2n$
 $hk0 : h, k=2n$
 $h00 : h=2n$
 $0k0 : k=2n$
 $00l : l=2n$

Special: as above, plus

8	<i>f</i>	$m..$	0, y, z	$0, \bar{y} + \frac{1}{2}, z + \frac{1}{2}$	$0, y + \frac{1}{2}, \bar{z} + \frac{1}{2}$	0, \bar{y}, \bar{z}
8	<i>e</i>	$.2.$	$\frac{1}{2}, y, \frac{1}{2}$	$\frac{1}{2}, \bar{y} + \frac{1}{2}, \frac{1}{2}$	$\frac{1}{2}, \bar{y}, \frac{1}{2}$	$\frac{1}{2}, y + \frac{1}{2}, \frac{1}{2}$
8	<i>d</i>	$2..$	$x, 0, 0$	$\bar{x}, \frac{1}{2}, \frac{1}{2}$	$\bar{x}, 0, 0$	$x, \frac{1}{2}, \frac{1}{2}$
8	<i>c</i>	$\bar{1}$	$\frac{1}{2}, \frac{1}{2}, 0$	$\frac{3}{2}, \frac{1}{2}, \frac{1}{2}$	$\frac{3}{2}, \frac{3}{2}, \frac{1}{2}$	$\frac{1}{2}, \frac{3}{2}, 0$
4	<i>b</i>	$2/m..$	$\frac{1}{2}, 0, 0$	$\frac{1}{2}, \frac{1}{2}, \frac{1}{2}$		
4	<i>a</i>	$2/m..$	0, 0, 0	$0, \frac{1}{2}, \frac{1}{2}$		

no extra conditions

 $hkl : h=2n$ $hkl : k+l=2n$ $hkl : k, l=2n$ $hkl : k+l=2n$ $hkl : k+l=2n$ **Symmetry of special projections**

Along $[001]$ $p2mm$
 $\mathbf{a}' = \frac{1}{2}\mathbf{a}$ $\mathbf{b}' = \frac{1}{2}\mathbf{b}$
 Origin at 0, 0, z

Along $[100]$ $p2gm$
 $\mathbf{a}' = \frac{1}{2}\mathbf{b}$ $\mathbf{b}' = \mathbf{c}$
 Origin at $x, 0, 0$

Along $[010]$ $p2mm$
 $\mathbf{a}' = \frac{1}{2}\mathbf{c}$ $\mathbf{b}' = \frac{1}{2}\mathbf{a}$
 Origin at 0, $y, 0$

Maximal non-isomorphic subgroups

I	[2] $C2ce$ ($Aea2$, 41)	(1; 4; 6; 7)+
	[2] $Cm2e$ ($Aem2$, 39)	(1; 3; 6; 8)+
	[2] $Cmc2_1$ (36)	(1; 2; 7; 8)+
	[2] $C222_1$ (20)	(1; 2; 3; 4)+
	[2] $C12/c1$ ($C2/c$, 15)	(1; 3; 5; 7)+
	[2] $C112_1/e$ ($P2_1/c$, 14)	(1; 2; 5; 6)+
	[2] $C2/m11$ ($C2/m$, 12)	(1; 4; 5; 8)+
IIa	[2] $Pmnb$ ($Pnma$, 62)	1; 3; 6; 8; (2; 4; 5; 7) + $(\frac{1}{2}, \frac{1}{2}, 0)$
	[2] $Pbca$ (61)	1; 3; 5; 7; (2; 4; 6; 8) + $(\frac{1}{2}, \frac{1}{2}, 0)$
	[2] $Pbna$ ($Pbcn$, 60)	1; 2; 3; 4; (5; 6; 7; 8) + $(\frac{1}{2}, \frac{1}{2}, 0)$
	[2] $Pmca$ ($Pbcm$, 57)	1; 2; 7; 8; (3; 4; 5; 6) + $(\frac{1}{2}, \frac{1}{2}, 0)$
	[2] $Pbnb$ ($Pccn$, 56)	1; 2; 5; 6; (3; 4; 7; 8) + $(\frac{1}{2}, \frac{1}{2}, 0)$
	[2] $Pmcb$ ($Pbam$, 55)	1; 2; 3; 4; 5; 6; 7; 8
	[2] $Pbcb$ ($Pcca$, 54)	1; 4; 6; 7; (2; 3; 5; 8) + $(\frac{1}{2}, \frac{1}{2}, 0)$
	[2] $Pmna$ (53)	1; 4; 5; 8; (2; 3; 6; 7) + $(\frac{1}{2}, \frac{1}{2}, 0)$
IIb	none	

Maximal isomorphic subgroups of lowest index**IIc** [3] $Cmce$ ($\mathbf{a}' = 3\mathbf{a}$) (64); [3] $Cmce$ ($\mathbf{b}' = 3\mathbf{b}$) (64); [3] $Cmce$ ($\mathbf{c}' = 3\mathbf{c}$) (64)**Minimal non-isomorphic supergroups****I** none**II** [2] $Fmmm$ (69); [2] $Pmcm$ ($\mathbf{a}' = \frac{1}{2}\mathbf{a}, \mathbf{b}' = \frac{1}{2}\mathbf{b}$) ($Pmma$, 51); [2] $Cmme$ ($\mathbf{c}' = \frac{1}{2}\mathbf{c}$) (67)

Contact

HEiDi

Phone: 089/289-14828

Web: <http://www.mlz-garching.de/heidi>

Martin Meven

Institut für Kristallographie Aachen, RWTH Aachen

JCNS Outstation at Forschungsneutronenquelle Heinz Maier-Leibnitz (FRM II)

Phone: 089/289-14727


e-Mail: Martin.Meven@frm2.tum.de

PANDA

Three-axis spectrometer

P. Link (TUM), A. Schneidewind

Jülich Centre for Neutron Science
Forschungszentrum Jülich

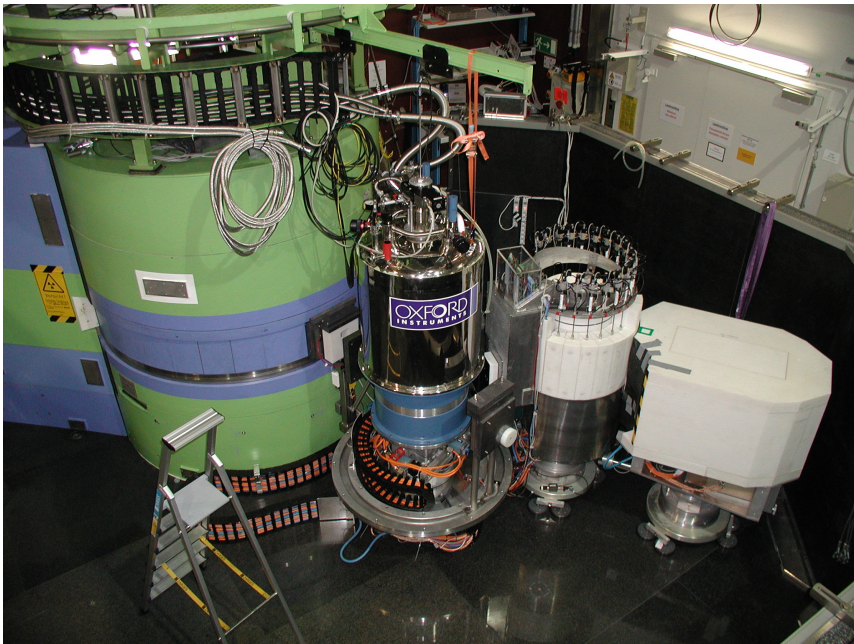

Contents

1	Introduction and theoretical basics	3
1.1	Inelastic scattering cross section	3
1.2	Elastic scattering function	3
1.3	Coherent vs. incoherent scattering	5
1.4	Reciprocal space and Brillouin-zones	5
1.5	Inelastic scattering processes	7
1.6	Dispersion relation	10
1.7	Transverse and longitudinal phonons	11
1.8	What is measured - what can we conclude for the sample	12
1.9	Normalization of the counting rates	15
1.10	Resolution function	16
1.11	Peak forms	17
2	Performance of the experiment	18
3	Experiment	23
4	Report	23
	Contact	26

1 Introduction and theoretical basics

This summary is thought as a repetition of the basic knowledge needed for this experiment. It is expected to be familiar with the different types of the crystal lattices, the terms of *unit cell* and *basis* as well as the use of *Miller's indices*.

1.1 Inelastic scattering cross section

In the experiment a sample is illuminated by a *monoenergetic* (energy E_i) neutron beam with a *direction* (wave vector \mathbf{k}_i). The ratio of the intensity scattered in a decent solid angle $d\Omega$ (wave vector \mathbf{k}_f) with the energy $E_f + dE$ to the intensity of the incoming beam is the differential scattering cross section

$$\frac{I_{\Omega, E_f}}{I_0} = \frac{d\sigma^2}{d\Omega dE_f}. \quad (1)$$

The scattering of the neutrons at the nuclei is handled within the quantum mechanics as a weak perturbation of the system. The calculation can be found as "Fermi's golden rule" in the textbooks. Reference: [6]

Generally, the scattering cross section is:

$$\frac{d^3\sigma}{d\Omega dE_f} = \frac{|\mathbf{k}_f|}{|\mathbf{k}_i|} S(\mathbf{Q}, \omega). \quad (2)$$

The scattering function S depends on the momentum transfer¹ $\mathbf{Q} = \mathbf{k}_i - \mathbf{k}_f$ and the energy transfer, to be written in a change of the wave length $\omega = \frac{E}{\hbar}$. The relation between ω or E and $|\mathbf{k}_f|$ is of squared, therefore the scattering cross section used in 1.9 is for the following calculations (Reference: [11], chap.4):

$$\frac{d^3\sigma}{d\mathbf{k}_{fx} d\mathbf{k}_{fy} d\mathbf{k}_{fz}} \propto \frac{1}{|\mathbf{k}_i|} S(\mathbf{Q}, \omega). \quad (3)$$

We start with elastic scattering ($|\mathbf{k}_i| = |\mathbf{k}_f|$). We will find that this is given by the assumption of a time-independent distribution of the scattering centers.

1.2 Elastic scattering function

We describe the incoming neutron beam as a plane wave. Its amplitude at every time t depends on the site $\mathbf{P} = \mathbf{R} + \mathbf{r}$ (see Fig. 1):

$$\mathcal{A}_P = \mathcal{A}_0 e^{i[\mathbf{k}_i \cdot (\mathbf{R} + \mathbf{r})] - i\omega_0 t}. \quad (4)$$

It excited the scattering centers to emit spherical waves with an amplitude \mathcal{A}' , having a fix phase relation to the original (incident) wave.

$$\mathcal{A}'_P = \rho(\mathbf{P}) \mathcal{A}_P, \quad (5)$$

¹ Really: the change of the wave vector. In units of \hbar this is exactly the momentum transfer.

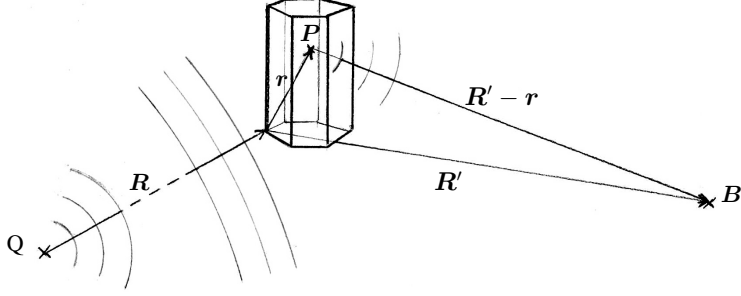


Figure 1: General scattering geometry and notation

$\rho(\mathbf{r})$ is the local scattering density with the unit m^{-2} . No multiple scattering occurs². At a site B we get for a wave starting from a site P :

$$\mathcal{A}_B(\mathbf{r}, t) = \mathcal{A}_P(\mathbf{r}, t) \rho(\mathbf{r}) \frac{e^{i[\mathbf{k}_f \cdot (\mathbf{R}' - \mathbf{r})]}}{|\mathbf{R}' - \mathbf{r}|} \quad (6)$$

where \mathbf{k}_f is pointing into the direction of $(\mathbf{R}' - \mathbf{r})$.

We assume the distance between R and R' to be large compared to r .

$$\mathcal{A}_B(\mathbf{r}, t) = \mathcal{A}_P(\mathbf{r}, t) \rho(\mathbf{r}) \frac{1}{R'} e^{i[\mathbf{k}_f \cdot (\mathbf{R}' - \mathbf{r})]} \quad (7)$$

with the same direction of \mathbf{k}_f for all P . After replacing \mathcal{A}_P and ordering:

$$\mathcal{A}_B(\mathbf{r}, t) = \frac{A_0}{R'} e^{i(\mathbf{k}_i \cdot \mathbf{R} + \mathbf{k}_f \cdot \mathbf{R}')} \rho(\mathbf{r}) e^{-i[(\mathbf{k}_f - \mathbf{k}_i) \cdot \mathbf{r}] - i\omega_i t}. \quad (8)$$

The first term is a constant phase factor, which is now space-independent within the sample. The whole scattering amplitude is given by integration of the scattering region.

$$\mathcal{A}_B(t) \propto e^{-i\omega_i t} \int_V \rho(\mathbf{r}) e^{-i[(\mathbf{k}_f - \mathbf{k}_i) \cdot \mathbf{r}]} d\mathbf{r}. \quad (9)$$

As long as ρ is time-independent, the time dependence of \mathcal{A}_B includes only the frequency ω_i (elastic scattering).

In the experiment, we do not have access to the amplitude of the wave but only to the square of it. For the scattering function one gets:

$$S(\mathbf{Q}) \propto \left| \int_V \rho(\mathbf{r}) e^{-i\mathbf{Q} \cdot \mathbf{r}} d\mathbf{r} \right|^2 \quad (10)$$

$$\text{with: } \mathbf{Q} = \mathbf{k}_f - \mathbf{k}_i. \quad (11)$$

Therefore, we identify the scattering function except a factor as the square of the Fourier transform of the scattering density. References: [7], [12]

² according to the Born approximation in the quantum-mechanical scattering theory

1.3 Coherent vs. incoherent scattering

Restricting on the interactions with the nuclei and using thermal neutron wavelengths ($\approx \text{\AA}$) which are large compared to the radii of the nuclei (10^{-4}\AA) the sample can be assumed to be an array of point-shaped scattering centers. The scattering density follows as:

$$\rho(\mathbf{r}) = \sum_i b_i \delta(\mathbf{r}_i - \mathbf{r}) \quad (12)$$

with the positions of the scattering centers \mathbf{r}_i and their scattering lengths b_i , respectively. b represents the amplitude of the spherical wave emitted by an atom and \bar{b} its average.

The scattering function of a material with identical atoms in regular order is again a regular point lattice (see next chapter). But, a normal crystal is a mixture of several isotopes having different neutron scattering lengths. In this case, the interference condition is valid only for an averaged scattering length. Taking (12) for (10), the scattering function is

$$S = (\bar{b})^2 S_{\text{coh.}} + (\bar{b}^2 - (\bar{b})^2) S_{\text{inc.}} \quad (13)$$

assuming a statistical distribution of the different scattering centers. $S_{\text{inc.}}$ is now independent of the relative positions of the atoms to each other and therefore independent of the concrete structure of the sample. It is a term of background signal, independent of the scattering angle and the sample orientation. This so-called incoherent scattering is always observed when the scattering density varies locally and non-correlated, also for point defects in the lattice and randomly distributed spin orientations in nuclei and atomic shells. A distinguished incoherent scatterer - almost without a coherent distribution - is vanadium which is often used for spectrometer alignments. Reference: [12]

1.4 Reciprocal space and Brillouin-zones

The samples to be investigated are normally good coherent scatterers, it is necessary to know $S_{\text{coh.}}$. Let's start on a Bravais-lattice with a one-atom basis. The scattering density is:

$$\rho(\mathbf{r}) = \sum_{h,k,l} b \delta^3[(h \mathbf{a}_1 + k \mathbf{a}_2 + l \mathbf{a}_3) - \mathbf{r}], \quad (14)$$

with generating lattice vectors \mathbf{a}_i . The Fourier transform of such a function is:

$$\tilde{\rho}(\mathbf{q}) = \frac{1}{\sqrt{2\pi}} \int \sum_{h,k,l} b \delta^3[(h \mathbf{a}_1 + k \mathbf{a}_2 + l \mathbf{a}_3) - \mathbf{r}] e^{-i\mathbf{q}\cdot\mathbf{r}} d\mathbf{r} \quad (15)$$

$$= \sum_{h,k,l} b e^{-i\mathbf{q}\cdot[h \mathbf{a}_1 + k \mathbf{a}_2 + l \mathbf{a}_3]}. \quad (16)$$

Summarizing for a sufficient number of indices, one gets a point lattice again, the *reciprocal lattice*³. The wave vector space is named the *reciprocal space*.

³ It can be shown that the reciprocal lattice of a Bravais lattice is a Bravais lattice again having all symmetry elements of the original lattice.

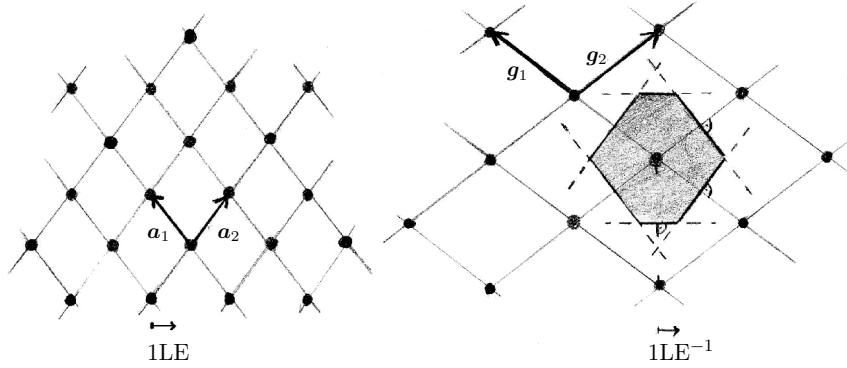


Figure 2: 2-dimensional point lattice in the real and reciprocal spaces. The first Brillouin zone is plotted around a reciprocal lattice point. Note the generating vectors of both lattices satisfying equation (17).

By

$$\mathbf{g}_i \cdot \mathbf{a}_j = 2\pi\delta_{i,j} \quad (17)$$

we get the generating vectors \mathbf{g}_i of the reciprocal space from the original vectors ⁴: The reciprocal lattice vector \mathbf{g}_1 is perpendicular to the vectors \mathbf{a}_2 and \mathbf{a}_3 with an absolute value of:

$$\frac{2\pi}{(a_1 \cos \angle(\mathbf{a}_1, (\mathbf{a}_2 \times \mathbf{a}_3)))}. \quad (18)$$

In the simple case of the sc lattice all real lattice vectors are pairwise perpendicular. Thus, the directions of the reciprocal space are identical to that of the real space. But, the dimensions of the reciprocal lattice as well as of the wave vectors are 'm⁻¹' (see eq. (17)).

In (10) we identified the scattering function as the square of the Fourier transformed of the scattering density. It is different from zero if

$$\mathbf{Q} = \mathbf{G} = h\mathbf{g}_1 + k\mathbf{g}_2 + l\mathbf{g}_3 \quad (\text{Laue condition}). \quad (19)$$


Wave vectors satisfying this condition built the Bragg reflections in the sample spectrum and are enumerated by the indices h, k, l .

fcc and bcc lattices are normally not presented by their primitive unit cells but as sc lattices with a polyatomic basis. Therefore, not all reflections of the sc lattice occur. This is described by the *structure factor*. Here eq. (17) does not give the generating wave vectors of the reciprocal space.


A useful construction to work with the wave vectors of the reciprocal space is the construction of the Brillouin zones. For this, in the reciprocal lattice the perpendicular bisector planes of the vectors connecting one lattice point with all the others are created. ⁵ (see also Fig. 2).

⁴ The definition (17) is used in physics. The 2π factor depends on the definition of the wave vector and is sometimes omitted, especially in crystallography.

⁵ All incoming plane waves with wave vectors ending at the Brillouin zone boundary satisfy the elastic scattering condition (19) since incident and final wave vector are of the same length.

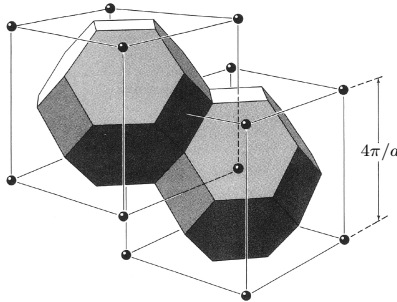

(a) The reciprocal lattice of a fcc crystals is a bcc lattice. The first two Brillouin zones are drawn. If the crystal consists of two interlocking fcc lattices (i.e. Silicon), not all reflections occur.

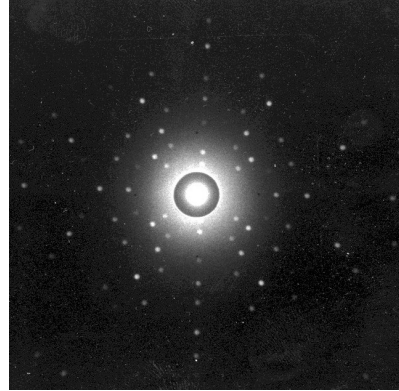

(b) Laue picture of a Silicon crystal ([110]-direction) irradiated by polychromatic x-rays. We get a two-dimensional projection of the reciprocal lattice up to decent indices, depending on the minimum wavelength of the x-rays.

Figure 3: 3-dimensional view of the elastic scattering.

Remark: The construction of the Brillouin zones is of the basis Bravais lattice. I.e., Germanium and Silicon have a fcc lattice with a 2-atomic basis. The scattering function is influenced in a way that several reflections vanish, others are amplified. The reciprocal lattice stays to be of fcc symmetry.

The first Brillouin zones around the points of the reciprocal lattice fill the reciprocal space. By this, points of high symmetry are easy to identify. They are used to be named by letters (see Fig. 6).

References: [7] Chapter about scattering on periodic structures.

1.5 Inelastic scattering processes

We allow a change of the scattering density ρ with time now.

$$\rho(\mathbf{r}(t)) \propto \sum_n \delta(\mathbf{r}_n(t) - \mathbf{r}). \quad (20)$$

The atoms are oscillating with weak amplitudes around their average position.

$$\mathbf{r}_n(t) = \mathbf{r}_n + \mathbf{u}_n(t). \quad (21)$$

Assuming the forces between neighboring atoms to be proportional to their displacement (harmonic approximation) every oscillation state of the crystal can be described as a superposition

of plane waves with wave vectors \mathbf{q} .⁶:

$$\mathbf{u}_n(t) = \sum_{\mathbf{q}} \mathbf{u} e^{\pm i(\mathbf{q} \cdot \mathbf{r}_n - \omega(\mathbf{q})t)}. \quad (22)$$

The scattering amplitude is from (10) and (20):

$$\mathcal{A} \propto e^{-i\omega_i t} \sum_n e^{-i\mathbf{Q} \cdot \mathbf{r}_n(t)}. \quad (23)$$

Take eq. (21) to develop the exponential function for small \mathbf{u} 's:

$$\mathcal{A} \propto e^{-i\omega_i t} \sum_n e^{-i\mathbf{Q} \cdot \mathbf{r}_n} e^{-i\mathbf{Q} \cdot \mathbf{u}_n(t)} \quad (24)$$

$$\approx e^{-i\omega_i t} \sum_n e^{-i\mathbf{Q} \cdot \mathbf{r}_n} [1 - i\mathbf{Q} \cdot \mathbf{u}(t)] \quad (25)$$

$$= e^{-i\omega_i t} \sum_{n,\mathbf{q}} e^{-i\mathbf{Q} \cdot \mathbf{r}_n} - i\mathbf{Q} \cdot \mathbf{u} e^{-i\mathbf{Q} \cdot \mathbf{r}_n} e^{\pm i(\mathbf{q} \cdot \mathbf{r}_n - \omega(\mathbf{q})t)}. \quad (26)$$

In (26) we find in addition to the terms from elastic scattering for every \mathbf{q} a term:

$$\sum_n i\mathbf{Q} \cdot \mathbf{u} e^{-i[(\mathbf{Q} \mp \mathbf{q}) \cdot \mathbf{r}_n] - i[\omega_i \pm \omega(\mathbf{q})]t}. \quad (27)$$

Thus, there are scattering waves with frequencies shifted from the frequency of the primary wave just by the frequency of the crystal oscillations. In addition, in analogy to the elastic case, the sum in (27) is non-zero only if eq.

$$\mathbf{Q} = \mathbf{k}_i - \mathbf{k}_f = \mathbf{G} \mp \mathbf{q} \quad (28)$$

is satisfied by a reciprocal wave vector \mathbf{G} . The condition for the frequency is:

$$\omega_f = \omega_i \pm \omega(\mathbf{q}). \quad (29)$$

Multiplying both equations with \hbar and choosing $\mathbf{G} = 0$ gives:

$$\hbar\Delta\omega \mp \hbar\omega(\mathbf{q}) = 0, \quad (30)$$

$$\hbar\mathbf{k}_f - \hbar\mathbf{k}_i \mp \hbar\mathbf{q} = 0. \quad (31)$$

This is just the quantum-mechanical description of the momentum and energy conservation for neutron scattering on a particle generally called a *phonon*. The analogy is confirmed also quantum-mechanically.

See i.e. [1] appendix N.

As to be seen from the equation, the momentum of a phonon is determined only modulo to one reciprocal lattice vector. Really two lattice oscillations of wave vectors differing by one

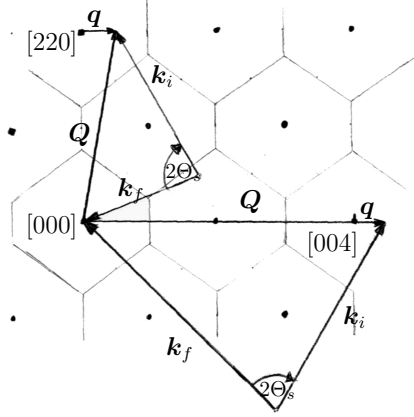


Figure 4: Scattering diagrams for inelastic scattering of neutrons on a fcc crystal. The reciprocal $[1\bar{1}0]$ plane is drawn. Notation similar to the text. The energy transfer is represented by the different lengths of k_i and k_f

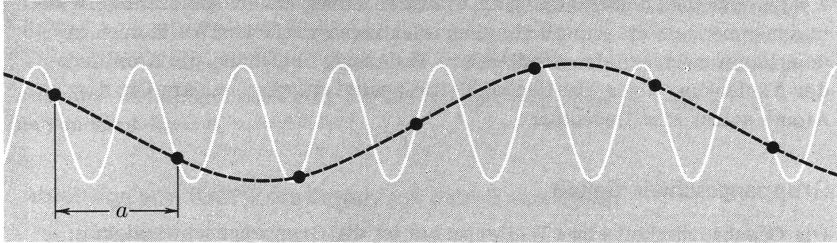


Figure 5: Equivalence of lattice vibrations taken from [9]: Both of the shown waves lead to the same displacement of the atoms from their average position. They are physically identical. All waves with a wavelength λ_1 smaller than $2a$ (white line) can be reduced to these with $\lambda_2 \geq 2a$ (black line). $\frac{2\pi}{\lambda_1} = \frac{2\pi}{\lambda_2} - n\frac{2\pi}{a}$, with $n\frac{2\pi}{a}$ the length of a reciprocal lattice vector. The waves with $\lambda \geq 2a$ are just these with wavevectors in the first Brillouin zone.

reciprocal lattice vectors are similar by physics (see fig. 5). Thus, the wave vector of every phonon can be related to the nearest reciprocal lattice point and the theoretical considerations are restricted to the 1. Brillouin zone. The probability of the excitation of a phonon scales with the intensity of the nearest elastic reflection. See for example fig. 9. Phonons are therefore particles with a quasi-momentum ⁷.

Reference: see [7] chapter 4

For the visualization of the inelastic scattering process one can assume that the neutron initiates an oscillation in the crystal. By this, the neutron loses energy or gains energy when scattered on an oscillating atom which results in the annihilation of this oscillation. For the energy loss, a decent mode has to be already excited in the crystal. Such a consideration of the energies leads to the "detailed balance" principle:

$$S(\mathbf{Q}, -\omega) = e^{-\frac{\hbar\omega}{k_B T}} S(\mathbf{Q}, \omega) \quad (32)$$

with the Boltzmann factor $k_B T$. At room temperature, both sides are almost equivalent.

What is now the advantage of neutrons for the study of lattice vibrations, compared to x-rays - which are easier to handle and available with much higher flux, especially at synchrotron sources where in addition higher brilliance is achieved? The energy of thermal neutrons is in average circa 30 meV which is related to a wavevector of 3.8 \AA^{-1} . The dimensions of the reciprocal space are given by eq. (17), i.e. circa 2 \AA^{-1} for Germanium. X-rays with similar wave vectors have energies of $\approx 10 \text{ keV}$. The excitation of a lattice vibration with an energy of 10 meV would be according to a relative energy change of 10^{-6} for photons. For neutrons the change is in the order of kinetic energies.

1.6 Dispersion relation

One purpose of the experiment is to determine the correlation $\omega(\mathbf{q})$ experimentally. $\omega(\mathbf{q})$ is the (phonon) dispersion relation. It contains all information about the dynamic properties of the studied material. Physical quantities as velocity of sound and the phonon contribution of the heat capacity can be deduced from it. But, also the dominating interaction potentials between the atoms can be derived. For the visualization the 3-dimensional relation is drawn for several directions of symmetry abreast.

The principle of $\omega(\mathbf{q})$ can be shown at an one-dimensional atomic chain. See the textbook derivation (i.e. [1]). The generalization is done by the transition to parallel crystal planes oscillating contrary.

⁶ This is the first-order Taylor series approximation of anharmonic potentials.

⁷ The real momentum transfer of the neutrons is - as for elastic scattering - absorbed by the whole sample and is not relevant due to the mass ratio.

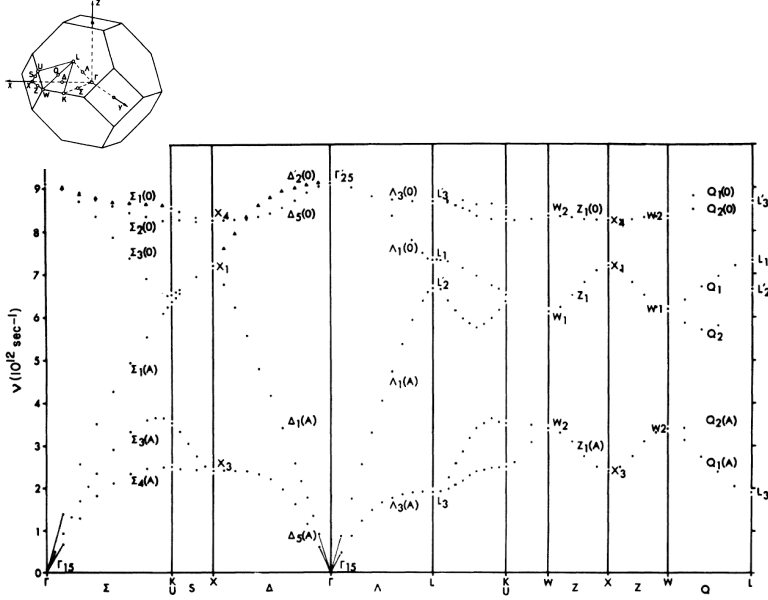



Figure 6: Dispersion relation of Germanium at 80 K taken from [10]. Points of exceptionally high symmetry are indicated by letters. (small picture).

1.7 Transverse and longitudinal phonons

As known from mechanics, for propagating waves the displacement of the single atoms can be chosen parallel (longitudinal) or perpendicular (transversal) to the propagation direction. In general, both excitations have different energies. For every \mathbf{q} there are two transverse phonons with polarizations perpendicular to each other, but only one of them is in the scattering plane. In crystals of high symmetry these excitations are degenerated in energy. A crystal with a one-atomic basis has three dispersion modes. For a basis of n atoms, this number increases to $3n$ (3 acoustic ($E = 0$ in the center of the B-zone) and $3(n - 1)$ optical modes ($E \neq 0$ at $q = 0$)). Fig. 6 shows this for the simple case of Germanium.

Reference: [9]

How can transverse and longitudinal oscillations be distinguished in the experiment? The equation of the inelastic scattering function (27) contains the scalar product $\mathbf{Q} \cdot \mathbf{u}$ with the polarization of the wave \mathbf{u} (fig. 7). Thus, an oscillation is only excited for \mathbf{Q} with a component in the polarization direction, in analogy to the classical assumption. Fig. 4 shows the measurement of a longitudinal and of a transverse phonon. The wave vector \mathbf{q} points in the same direction for both measurements.

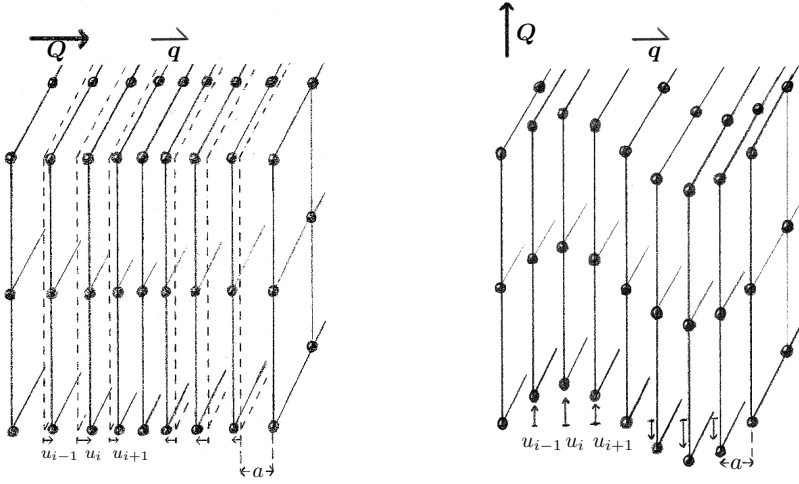

(a) longitudinal . . .

(b) and transversal oscillations

Figure 7: Note: The momentum transfer of the neutrons Q points always into the direction of the real displacements u_i .

1.8 What is measured - what can we conclude for the sample

We look now at the correlation between the configuration of the spectrometer and the variables Q and ΔE . The absolute values of k_i and k_f (incident and outgoing wave vectors) are determined by the scattering angles at the monochromator and the analyzer crystals $2\Theta_m$ and $2\Theta_a$, respectively⁸. Having neutron waves we need

$$E_{\text{kin}} = \frac{(\hbar k_n)^2}{2m}, \quad (33)$$

with p the momentum and m the mass of the neutron.

Thus, we know also


$$\omega = \frac{\Delta E}{\hbar} = \hbar \frac{|\mathbf{k}_i|^2 - |\mathbf{k}_f|^2}{2m_n}. \quad (34)$$

The orientation of the sample determines the direction of \mathbf{k}_i relatively to the crystal lattice (characterized by the sample rotation angle ω_s) and the scattering plane. Within the scattering plane $2\Theta_s$ determines the direction of \mathbf{k}_f . Q results from eq. (11).



Conversely, we do not get the configuration of the instrument from ω and Q .

In standard experiments, the scans are done at constant Q or constant energy transfer ΔE . While for very stiff dispersion modes, in the vicinity of the Brillouin zone center, constant- E is chosen (Fig. 8(b)), most of the Brillouin zone is normally measured with const.- Q (Fig. 8(a)).


⁸ $2\Theta_m$ and $2\Theta_a$ are the relevant numbers. The rotation of the crystals Θ_m and Θ_a are fixed in relation to $2\Theta_m/2$ and $2\Theta_a/2$.

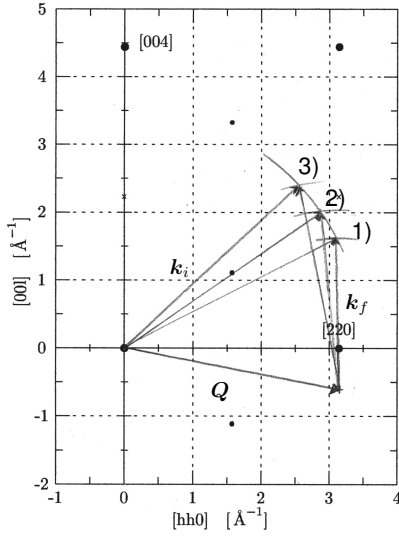

(a) Example for constant- Q scans

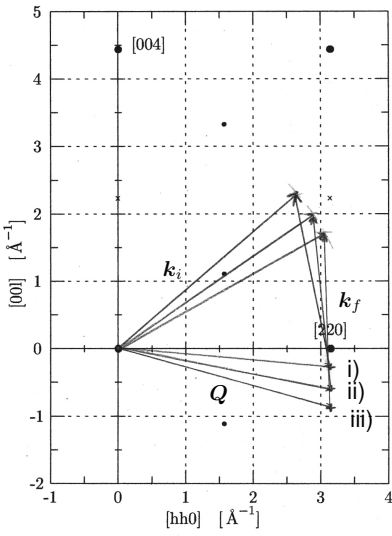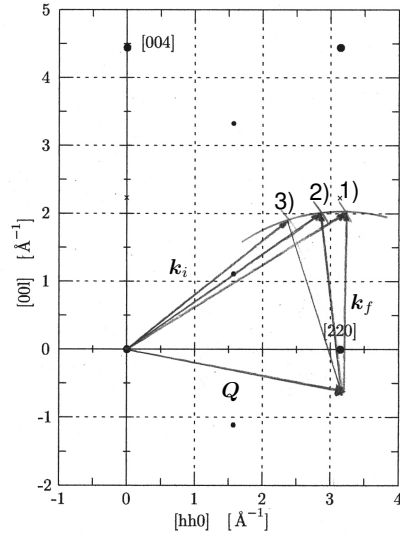

(b) A constant- E scan

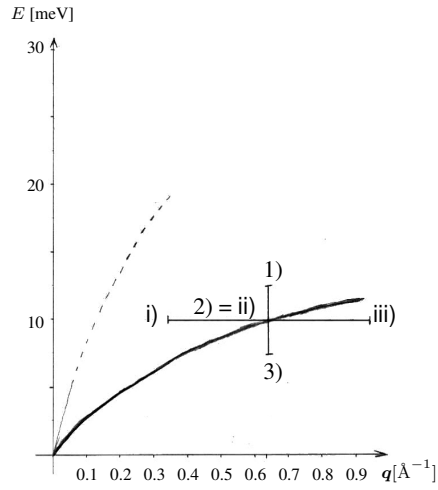

(c) corresponding points of the dispersion relation

Figure 8: Examples for different scans (scattering triangles and dispersion relation.)

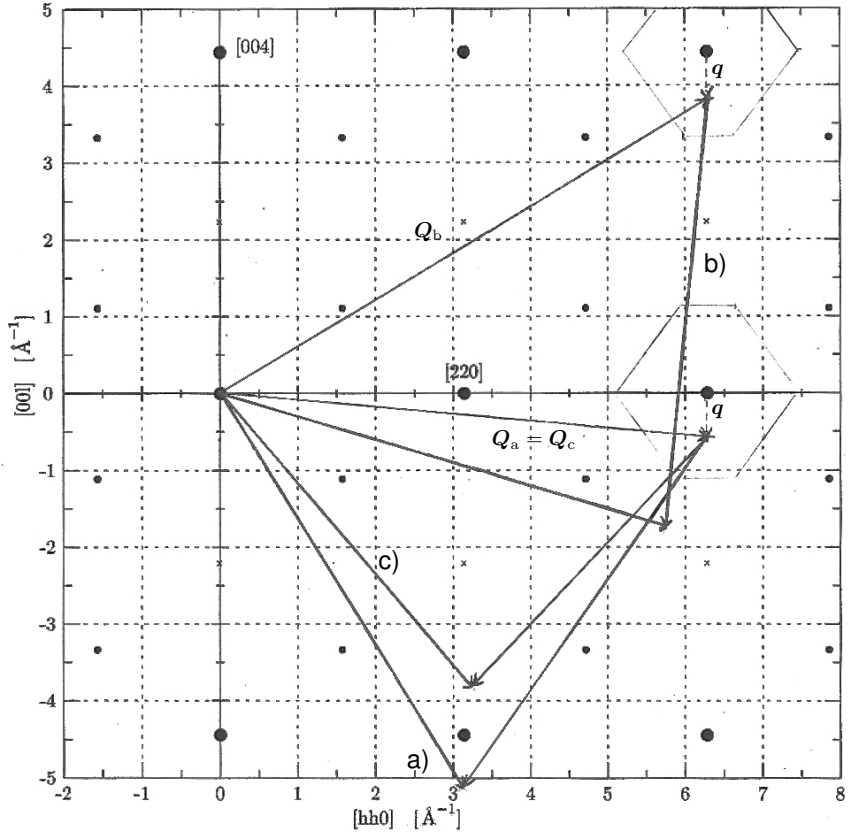


Figure 9: The same phonon excitation measured in different ways:

(a) \leftrightarrow (b): Measurements at different elastic peaks but with identical $|\mathbf{k}_i|$ and $|\mathbf{k}_f|$.

(a) \leftrightarrow (c): Identical position of the reciprocal space measured with different \mathbf{k}_i .

Please take time and think about the reason and how the different angles change during the two measurements shown in the figures.

As demonstrated in fig. 9, the lengths of \mathbf{k}_i or \mathbf{k}_f can be fixed. This is a way to change the resolution of the instrument optimizing the measurement for different problems.

1.9 Normalization of the counting rates

Planning an experiment, it seems to be native to count the scattered neutrons in the detector at every point for a useful time. But, the counting rate Z_{Det} depends not only on the scattering cross section. It also depends on instrument parameters which possibly change during the measurement or within a scan.

$$Z_{\text{Det}} \propto I_{\text{prim}}(\mathbf{k}_i) \cdot R_{\text{Mono}}(|\mathbf{k}_i|) \frac{d^3\sigma}{d\mathbf{k}_{fx} d\mathbf{k}_{fy} d\mathbf{k}_{fz}} R_{\text{Anal}}(|\mathbf{k}_f|) \cdot P_{\text{Det.}}(|\mathbf{k}_f|) \quad (35)$$

$$= I_{\text{prim}}(\mathbf{k}_i) \cdot R_{\text{Mono}}(|\mathbf{k}_i|) \frac{1}{|\mathbf{k}_i|} S(\mathbf{Q}, \omega) R_{\text{Anal}}(|\mathbf{k}_f|) \cdot P_{\text{Det.}}(|\mathbf{k}_f|). \quad (36)$$

with $R(|\mathbf{k}|)$ the reflectivities of the Bragg crystals, $P_{\text{Det.}}(|\mathbf{k}_f|)$ the efficiency of the detector and $I_{\text{prim.}}(|\mathbf{k}_i|)$ the incident intensity at the used energy.

In our experiment here we are especially interested at the *positions* of the phonon excitations in the \mathbf{Q} - ω space and not too much in their intensities. We therefore do not ask for the comparability of *different* scans. We only need sufficient count rates *within* the scans and possibly the normalization of different points in a scan to determine the peak position in a right way.

We use a monitor detector usually mounted after the monochromator and before the sample. The probability to be detected is for neutrons with a velocity v proportional to the time t the neutrons stay in a detector (monitor) of the width d :

$$t = \frac{d}{v} = \frac{d m_n}{\hbar |\mathbf{k}|} \quad (37)$$

One expects as monitor count-rate:

$$Z_{\text{Mono}} \propto I_{\text{prim}}(\mathbf{k}_i) \cdot R_{\text{Mono}}(|\mathbf{k}_i|) \frac{1}{|\mathbf{k}_i|} \quad (38)$$

To perform a measurement, events are counted in the detector until a particular number of monitor counts is reached. The real count rate in the detector with monitor Z'_{Det} is:

$$Z'_{\text{Det}} = \frac{Z_{\text{Det}}}{Z_{\text{Moni}}} \propto S(\mathbf{Q}, \omega) R_{\text{Anal}}(|\mathbf{k}_f|) \cdot P_{\text{Det.}}(\mathbf{k}_f). \quad (39)$$

For constant $|\mathbf{k}_f|$, as illustrated in fig. 8(a)(right), this dependence vanishes. This is therefore the common mode. If $|\mathbf{k}_f|$ is varied by any reasons during the scan, the corresponding corrections have to be done for the data analysis.

1.10 Resolution function

Up to now we did not consider the fact that at every point of the \mathbf{Q} - ω -space the spectrometer is pointing to the measured intensity is scattered in a finite volume around this point. A sharp (δ -) peak in the scattering function at (\mathbf{Q}_0, ω_0) gives a measured signal of the form:

$$Z_{\text{Det}}(\mathbf{Q}, \omega) \propto R(\mathbf{Q} - \mathbf{Q}_0, \omega - \omega_0). \quad (40)$$

R is the *resolution function* and depends on the configuration of the spectrometer only. Ordinary R is assumed to be Gaussian in its components.

The measured signal results from the convolution:

$$Z_{\text{Det}}(\mathbf{Q}, \omega) \propto \int S(\mathbf{Q}', \omega') R(\mathbf{Q}' - \mathbf{Q}, \omega' - \omega) d\mathbf{Q}' d\omega'. \quad (41)$$

For illustration take a contour line of the resolution function (exactly: the 2-dimensional projection of the resolution function). It is normally elliptically and shows the region of the scattering function 'seen' by the instrument. In fig. 10 the projections of the resolution function are plotted into the dispersion relation, at the right the intensities to be expected, respectively. A measurement is characterized to be *focused* if the short axes of the resolution ellipsoid is perpendicular to the dispersion surface (to be measured).

It is important to understand in which cases a sharp resolution function is helpful or not. E. g., see a const.- \mathbf{Q} -scan through a sharp 'horizontal' dispersion surface:

$$S(\mathbf{Q}, \omega) = S_0 \delta(\omega - \omega_0). \quad (42)$$

The measurement is focused, i.e.

$$R(\mathbf{Q}, \omega) = e^{-\frac{\omega^2}{\sigma_\omega}} \cdot R(\mathbf{Q}). \quad (43)$$

Eq.(41) gives:

$$Z(\omega) \propto e^{-\frac{\omega^2}{\sigma_\omega}} \int R(\mathbf{Q}) d\mathbf{Q}. \quad (44)$$

Expanding the resolution ellipsoid in the momentum coordinates, the measured intensity increases. The line width depends only on $e^{-\frac{\omega^2}{\sigma_\omega}}$.

Reference: [11] Chap.4

The real form of the resolution function is influenced now by several effects: The Bragg-crystals are not of perfect lattices but have a finite mosaicity (which means it consists of several small single crystals, and their lattice parameters have weak deviations from the average). This 'mosaicity spread' - given by the angle η_m - broadens the Bragg peaks e.g. at the monochromator. Further influences are the finite angle resolution of the detectors, a finite size of the sample and diverging beams.

The beam reflected at the monochromator is a bunch of wave-vectors with a distribution $p_m(\mathbf{k}_i)$, the transmission function of the monochromator. The analyzer has to be described in analogy.

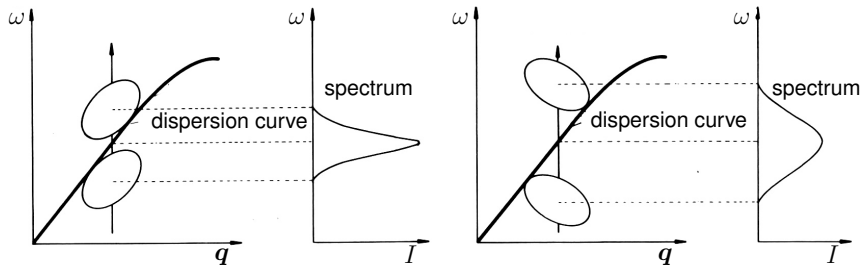


Figure 10: Focused vs. unfocused measurement.

To calculate the resolution function of the spectrometer, the two transmission functions have to be convoluted with respect to $2\Theta_s$. This simulation can be done by software tools. You will get some qualitative ideas about this within the experiment.

Reference: [4]

1.11 Peak forms

We learned: For sharp peaks in the scattering function we get a Gaussian signal in the measurement. This will be found in most of the experiments. However, some compounds exhibit broadened phonon resonances, so-called *soft modes*. They are originated by phonon-phonon- and phonon-electron-interactions⁹ and result in a finite lifetime τ of the single oscillation states. Calculating the damped harmonic oscillator the line shape is identified to be Lorentzian:

$$S(\omega) \propto \frac{\omega^2}{(\omega_0^2 - \omega^2)^2 + \left(\frac{\omega}{\tau}\right)^2} \quad (45)$$

with the line width (FWHM):

$$\delta\omega = \frac{1}{2\tau}. \quad (46)$$

The resulting signal of such a 'soft' peak is the convolution of a Lorentzian with a Gaussian curve called Voigt profile. This profile is not easy to be calculated mathematically. In the case of comparable widths of the single profiles it can be sufficient to take the width of the Voigt curve as the sum of the widths of the Gaussian and the Lorentzian contributions.

If it is necessary for the data analysis to determine the peak *widths*, the resolution function has to be deconvoluted from the measured signal. This can be done by software.

Reference: [3], [5]

⁹ These effects are neglected by the assumption of harmonic oscillations.

2 Performance of the experiment

PANDA is a three axis spectrometer (TAS) at the cold source of FRM II. The first thermal TAS was built 1954 and generally improved 1959 by Bertram N. Brockhouse at NRU Reactor in Chalk River. For his merit in the field of inelastic neutron scattering he got the Nobel price 1994. Even if the intensities at the detector were increased by magnitudes, the instrument is remote controlled and the safety is improved today, the general principle of the method is still the same:

The beam of cold neutrons (energy $E \approx 5(30)$ meV, momentum $p \approx 1.5(4) \cdot 10^{-24}$ kg m/s), which has de Broglie wavelength

$$\lambda = \frac{h}{p}, \quad (47)$$

or a wavevector of the length $k = \frac{2\pi}{\lambda}$, exits the moderator tank of the reactor through a beam port. The neutrons enter a monochromator being of single crystals with a d-spacing d .

By the Bragg equation

$$n\lambda = 2d \sin \Theta_m \quad (48)$$

the angle $2\Theta_m$ defines the energy of a monochromatic neutron beam (wave vector \mathbf{k}_i , energy E_i), which points to the sample to be investigated.

Direction and energy of the neutrons are changed at the sample following the inelastic scattering laws. At the secondary spectrometer (analyzer) neutrons with the wave vector \mathbf{k}_f and the energy E_f are selected by Bragg reflection at a second crystal and are counted in the detector. By this, the momentum transfer (\mathbf{Q}) of the neutrons to the sample as well as the energy transfer (ΔE) from the sample to the neutrons can be determined.

$$\mathbf{Q} = \mathbf{k}_i - \mathbf{k}_f, \quad \Delta E = E_i - E_f. \quad (49)$$

For useful statistics normally a fixed configuration of the instrument - related to a decent energy and momentum transfer - is taken for counting at the detector. The scattering function of the sample is therefore taken pointwise. These scans are measured at constant \mathbf{Q} or at constant energy E , depending on the experimental strategy (see below).

PANDA is located at the beamport SR2 in the experimental hall of FRM II and has a comparably large neutron flux at low background. For more detail see:

<http://www.mlz-garching.de/panda>.

We now discuss the components of the three axis spectrometer. Photos of the main components are collected at the gallery 22 for better understanding.

Shielding Since neutrons damage biological matter the region of the primary beam has to be shielded. This is done by a so-called drum (in the case of PANDA blue / green colored) with the monochromator in its centre. The drum is made of heavy concrete with a large amount of chemically combined water, boron added. Also used are boron-treated (PE) sheets. Chemically combined water and PE contain a large amount of hydrogen which is able to decelerate fast

Notation:

\mathcal{Q}	Neutron source
\mathcal{M}	Monochromator
\mathcal{S}	Sample table
\mathcal{A}	Analyzer
\mathcal{D}	Detector
α_1	collimators
α_2	
α_3	
α_4	
$2\Theta_m$	angles of the
$2\Theta_s$	Spectrometer-
$2\Theta_a$	axis
Abs	Shielding
Sel	Selector
Mob	Mobile blocks
Sh	Primary shutter

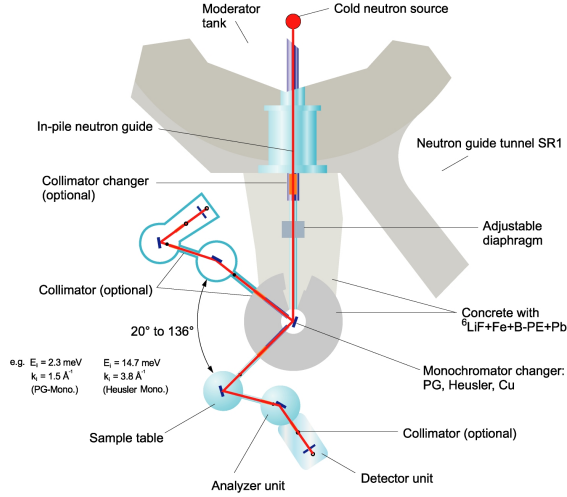


Figure 11: Schematic design of a three axis spectrometer.

Remark: all angles are counted in the region $[-180^\circ, 180^\circ]$. (0° is directed in beam, positive angles are counter-clockwise.) $2\Theta_s$ is therefore positive.

neutrons. Boron as a large absorption coefficient for cold and thermal neutrons¹⁰, and the isotope emerging at the neutron capture is not radioactive. But, normally materials are activated by the nuclear reactions and therefore activated (and the reactor emits hard Gamma radiation also if the primary shutter is closed), so the shielding has to be opened only after measurements of the remaining radiation even if the reactor is down. A part of the installation is shown here at the photos. The drum is made to shield γ -radiation as well as neutrons.

During the movement of the monochromator axes a ring of the shielding which contains the beam channel for the beam scattered at the monochromator is entrained. To avoid a closing of the primary beam during the ongoing rotation, the ring partially consists of 11 so-called mobile blocks (made of the same concrete as the ring) which are moved by an automatic control from one side of the opening to the other. The geometry and the control ensure a proper shielding where necessary (see fig.11).

Monochromator In the rotation centre of the shielding the monochromator is positioned. It consists of 121 single crystals of pyrolytic graphite (PG) mounted on a crystal holder. The crystal holder and therefore the graphite lattice planes are rotated by the angle Θ_m to the primary beam. The intensity of the monochromatic beam scattered at the angle $2\Theta_m$ ¹¹ depends on the lattice parameter of the monochromator material (here PG) and on the incoming angle..

To avoid contamination of higher-order Bragg reflection in the incoming beam, $n = 2, 3, \dots$ (Gl. (48)), filter materials are positioned between monochromator and sample. In the case of

¹⁰ Typical reaction: ${}^{10}_5\text{B} + {}^1_0\text{n} \rightarrow {}^3_3\text{Li} + {}^4_2\text{He} + 2.8 \text{ MeV}$

¹¹ Remark: Sometimes the angles Θ_m , Θ_s and Θ_a are named α_1 to α_3 .

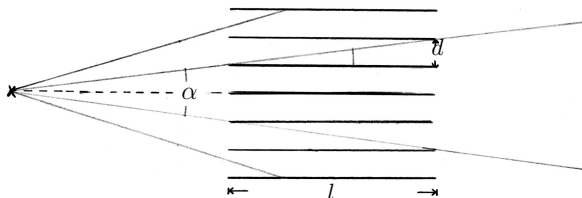


Figure 12: Drawing of a Soller collimator. The divergence of the outgoing beam is $\tan(\alpha/2) = d/l$, which is in the example ca. 18° . On PANDA the collimation can be chosen between 15 and 80 minutes.

PANDA this is polycrystalline boron or, sometimes, pyrolytic graphite.

Maximum intensity at sample and detector can be achieved by focusing the monochromator and the analyzer in horizontal and vertical direction. Here the 121 monochromator (55 analyzer) crystals are curved in both directions by complex mechanics to get the crystal surfaces into a paraboloid-like shape. The radius of the curvature depends on the neutron wavelength. By taking into account the distances also a focus of the momentums is possible.

Sample table The sample is mounted on a table which can be moved on air-pressure. In addition to motors rotating the sample and the analyzer/detector around the sample - giving Θ_s and the scattering angle $2\Theta_s$, the sample orientation can be adjusted by goniometers and translation stages. For studies of magnetism, the sample is normally positioned in a cryostat or a cryomagnet - cooling down to temperatures of 0.03 K and applying fields up to 13.2 T.

Analyzer The analyzer is also located in a shielding, but here the reason is to decrease the background in the detector. The crystal holder located again on a goniometer and translation stages allows a horizontal focus of the analyzer, the crystals are mounted to have a fixed vertical focus. The crystals are at the angle Θ_a to the beam, the detector is rotated by $2\Theta_a$.

Detector The neutrons are counted by a beamtube, filled with ^3He under high pressure (ca 10 bar). A neutron can be trapped by a ^3He nucleus and converted to ^4He . The emitted γ quant ionize the gas and is detected like in a Geiger-Müller counter. This allows to count ca. 90% of the incoming neutrons.

Diaphragms, collimators and attenuators In addition to the already described parts several components are needed in the beam path for beam conditioning. For example variable diaphragms (slits) are installed before and after the sample which are adjusted to the sample size to decrease the background. A secondary shutter is mounted after the monochromator. More diaphragms are with the primary shutter in the reactor wall and between the primary shutter and the monochromator.

Beyond that in every part of the beam path so-called Soller collimators can be applied. It con-

tains of ca. 20 cm long, coated with white GdO_2 foils, which are exactly parallel and therefore limit the divergence of the beam. The value of the divergence is described by the angle α (see fig. 12). Collimators with $\alpha = 15'$ to $\alpha = 60'$ are available. Small divergence corresponds with high resolution but small intensity. The primary collimators are placed in the primary shielding and are changed automatically, the others have to be changed by hand (motorization planned). The beam size is limited only horizontally, i.e. within the scattering plane. For increase of intensity we normally allow a large divergence of the beam in the direction perpendicular to the scattering plane.

Sometimes, e.g. for alignment, the detector is in the straight beam or Bragg reflections have a very large intensity. To avoid a saturation of the detectors, the incoming beam is attenuated by PE-plates of different thicknesses which can be moved into the beam (and combined) automatically.

Monitor To compare or to combine data from different scans or measurements the intensities are normalized to an intensity counted by the monitor in the primary beam. Its signal is proportional to the incoming intensity. This is also important for energy scans, where the incoming intensity changes with $2\Theta_m$ due to the energy-dependent spectrum. Also different reactor power can be corrected in this way (see paragraph 1.9).

Goniometer Monochromator, analyzer and sample are placed on 2-axis goniometers. This allows tilts around two perpendicular to each other which meet in the centre of the beam. So the sample does not move out of the beam centre during the tilt. The available angles are limited ($\pm 15^\circ$), the sample can be adjusted but has to be pre-oriented before measuring on the three-axis instrument. It is also possible to translate the sample a few millimeters horizontally and vertically.

Cover page: Overview over PANDA

From left: Monochromator shielding, sample table with 15T cryomagnet, analyzer box and detector shielding.


Figure 13: *(Following page) Components of PANDA taken in different phases of the construction.*



(a) Side view into the (opened) Monochromator shielding onto the PG-monochromator.



(b) PG-analyzer in the (opened) analyzer box. The horizontal curvature is changed by rotating the individual segments.

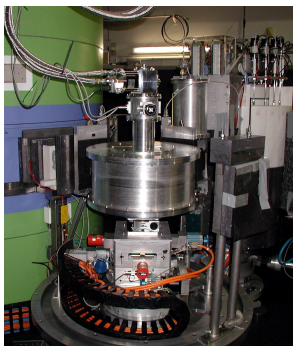

(c) Detailed view onto the sample table with vacuum chamber. From bottom: Rotation table, xy-stage, goniometer, z-stage



(d) Soller collimators in the automatic changer for α_1 (in the primary beam.)



(e) Typical sample mounting for use of cryostat.



(f) Detector tubes to be built into the detector shielding

3 Experiment

PANDA is a complex research instrument, where normally measurements on samples at very low temperature, high magnetic fields and / or high pressure are performed. Phonons for example are measured to learn about the interaction potentials in solids. Measurements of spin wave dispersions contribute to determine magnetic interactions.

The goal of this practice is to give inside to the potential of neutron scattering on a three-axis spectrometer. To get results, you have to understand the functionality of the instrument. This can include the alignment of the instrument and the sample. Some data can be taken on a well-known sample, e.g. lead, which can be measured at room temperature (necessary due to the limited time of the practice. A normal experiment needs several days.)

1. Preparation

- Gather theoretical basics.
- Generate a strategy for the measurements and a plan of the experiment.
- Safety instruction at the instrument PANDA.

2. Alignment

- Proof of the instrument alignment by scans of the monochromator or analyzer axis
- Determination of the (energy) resolution of the spectrometer for (min.) three different wave vectors by measuring of the incoherent elastic intensity on vanadium. Choose an appropriate configuration for the following measurements.
- Alignment of the sample, define the scattering plane, optimize background.
- Perform control scans and learn the use of the user interface on PANDA.

3. Measurements

- Perform the planned scans to determine the resolution ellipsoid.
- Measure (min.) one mode of the dispersion relation of lead by different scans.

4 Report

After the experiment you have to report your work. Please explain the experiment and your work in a short way to show how you understand the aim of the different steps. You can prepare this by doing notes during the experiment.

Please analyze the data and interpret it. It is not necessary to repeat the theoretic aspects already discussed in front of the experiment. But your report should be conclusive.

Please:

- Show the measured energy resolution depending on the wave vector. Explain your choice.

- Determine the direction of the resolution ellipsoid, add it to a scheme of the dispersion and show the single scans.
- For the measurements of lead, plot the measured points with the error bars into a dispersion relation(s) and compare to references. Explain how different scan types influence the result.

Finally: please give us a short feedback about the preparation, experiment and support. This can also be done after the experiment. We like to give you an impression about neutron scattering experiments even if practices are complicated. A feedback will help us to improve it for future students.

P.S. Do not forget ruler and calculator.

References

- [1] N. W. Ashcroft and N. D. Mermin. *Festkörperphysik*. Oldenbourg, 2001.
- [2] B. N. Brockhouse and P. K. Iyengar. Normal modes of germanium by neutron spektrometry. *Phys. Rev.*, 111(3):747, Aug 1958.
- [3] W. Demtröder. *Laserspektroskopie*, Kapitel 3 (Linienbreiten und Profile von Spektrallinien). Springer, 4. edition, 2000.
- [4] B. Dorner. *Coherent Inelastic Neutron Scattering in Lattice dynamics*. Springer-Verlag, 1982.
- [5] K. Dransfeld, P. Kienle, and G. M. Kalvius. *Physik I*, Kapitel 8. Oldenbourg, 8. edition, 1998.
- [6] H. Friedrich. *Theoretische Atomphysik*. Springer, 1990.
- [7] H. Ibach and H. Lüth. *Festkörperphysik, Einführung in die Grundlagen*. Springer-Verlag, 6. edition, 2002.
- [8] J. Kauppinen and J. Partanen. *Fourier Transforms in Spectroscopy*. Wiley-VCH, Berlin, 2001.
- [9] C. Kittel. *Einführung in die Festkörperphysik*. Oldenbourg, 10. edition, 1993.
- [10] G. Nillson and G. Nellin. Normal vibrations of germanium by neutron spektrometry. *Phys. Rev. B*, 3(2):364, Jan 1971.
- [11] G. Shirane, S. m. Shapiro, and J. M. Tranquada. *Neutron scattering with a triple-axis Spektrometer*. Oxford University Press, 2002.
- [12] B. T. Willis, editor. *Chemical Applications of Thermal Neutron Scattering*. Oxford University Press, 1973.
- [13] R. Zorn. Fourier transforms. In *Neutron Scattering*. T. Brückel, G. Heger, D. Richter and R. Zorn, 2006.

Internet resources

<http://http://www.mlz-garching.de/panda>
"PANDA" homepage.

<http://www.env-it.de/umweltdaten/>
Environmental data from the federal Ministry for the Environment, Nature Conservation and Nuclear Safety.

<http://www.umweltdaten.de/utk/kapitel22/E-22-1-2.pdf>
Estimations of natural and civil exposure in Germany from 1999.

Contact

PANDA

Phone: 089/289-14749

Web: <http://www.mlz-garching.de/panda>

Astrid Schneidewind

JCNS at Maier-Leibnitz Zentrum Garching, Forschungszentrum Jülich GmbH

Phone: 089/289-14749

e-Mail: Astrid.Schneidewind@frm2.tum.de

Petr Cermak

Phone: 089/289-11773


e-Mail: p.cermak@fz-juelich.de

SPHERES

Backscattering spectrometer

J. Wuttke

Jülich Centre for Neutron Science
Forschungszentrum Jülich

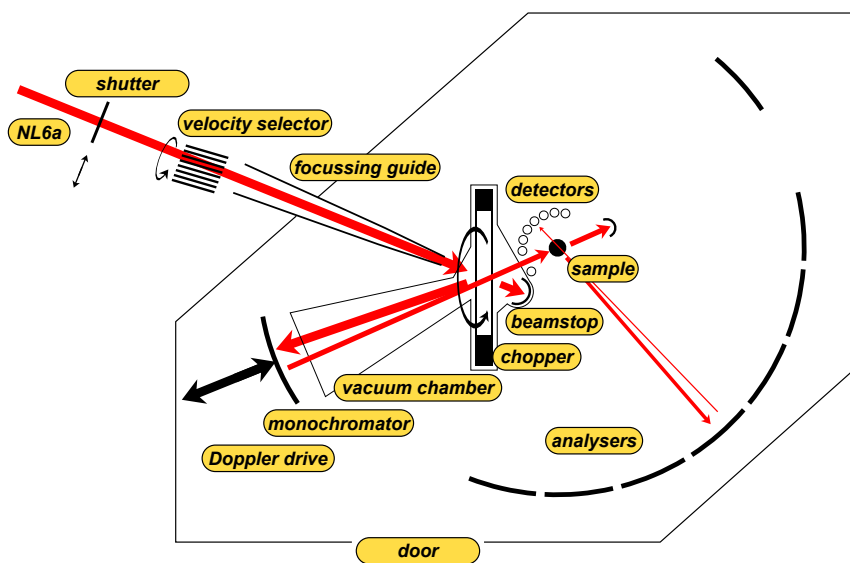

Contents

1	Introduction	3
2	Spectrometer Physics	3
2.1	Energy Selection by Backscattering	3
2.2	Spectrometer Layout	5
2.3	Measuring Spectra	7
2.4	Instrument Characteristics	7
3	Applications	8
3.1	Hyperfine Splitting	8
3.2	Molecular Rotation and Quantum Tunneling	9
4	Preparatory Exercises	11
5	Experiment Procedure	12
5.1	The experiment itself	12
5.2	Raw data reduction	12
5.3	Data evaluation	12
	Contact	14

1 Introduction

Neutron *backscattering spectrometers* are used to measure *inelastic scattering* with very high *energy resolution*. What does this mean?

In inelastic scattering, scattering intensity is measured as function of the energy exchanged between the scattered neutron and the sample. As in other areas of physics, a data set of the form intensity-versus-energy is called a *spectrum*. An instrument that resolves inelastic scattering is therefore called a *spectrometer*.

While elastic scattering experiments yield information about *structure* or *texture* of a sample, inelastic scattering is used to investigate its *dynamics*. Specifically, inelastic neutron scattering yields information about the thermal motion of atomic nuclei.

The most common instrument for inelastic neutron scattering is the triple-axis spectrometer. It is routinely used to measure phonon and magnon dispersions, with energy exchanges of the order of meV. In contrast, the *high resolution* of a backscattering spectrometer allows to resolve very *small energy shifts* of the order of μeV . By the time-energy uncertainty relation, small energy means long times. Hence, backscattering addresses relatively *slow* nuclear motion — much slower than the lattice vibrations typically seen in triple-axis spectrometry.

What processes take place on the energy or time scale made accessible by neutron backscattering? For instance the following:

- »hyperfine splitting of nuclear spin orientations in a magnetic field,
- »rotations or hindered reorientations of molecules or molecular side groups,
- »quantum tunneling,
- »hydrogen diffusion in solids,
- »relaxation (molecular rearrangements) in viscous liquids,
- »innermolecular rearrangements in polymers.

During your lab course day, you will use the backscattering spectrometer SPHERES (SPectrometer for High Energy RESolution) to study one example of these applications.

2 Spectrometer Physics

2.1 Energy Selection by Backscattering

In crystal spectrometers, neutron energies are selected by Bragg reflection from crystals, according to the *Bragg condition*

$$n\lambda_n \approx 2d_{hkl} \sin \theta \quad (1)$$

where d_{hkl} is the distance of lattice planes $\{hkl\}$, and θ is the glancing angle of reflection from these planes. The index n indicates that along with a fundamental wavelength λ_1 , integer fractions $\lambda_n \approx \lambda_1/n$ are transmitted as well. To suppress these unwanted higher orders, experimental setups include either a mechanical neutron velocity selector (Fig. 1), or a beryllium filter.

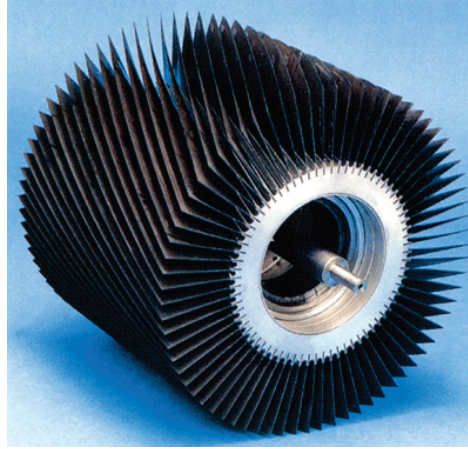


Fig. 1: Rotor of a mechanical neutron velocity selector. The blades are coated with neutron absorbing material. In SPHERES, such a selector is used as a pre-monochromator that reduces the incoming white spectrum to about 0.7%. © Astrium GmbH.

In practice, the parameters d and θ on the right-hand side of Eq. (1) are not sharp: Imperfections of the crystal lead to a distribution of lattice constants, characterized by a width δd . And similarly, imperfections of the neutron optics (inevitable because the incoming beam, the sample, and the detector all have finite size) lead to a distribution of reflection angles, characterized by a width $\delta\theta$. By differentiating the Bragg equation (1), one obtains the relative width of the wavelength distribution reflected by a crystal monochromator:

$$\frac{\delta\lambda}{\lambda} \approx \cot(\theta) \frac{\delta d}{d} + \frac{\delta\theta}{\theta} \quad (2)$$

In usual crystal spectrometers, the second term is the dominant one. However, by choosing $\theta \approx 90^\circ$, the prefactor $\cot(\theta)$ can be sent to zero. This is the fundamental idea of the backscattering spectrometer. If a monochromator crystal is used in backscattering geometry, with $\theta \approx 90^\circ$, then the reflected wavelength distribution is in first order insensitive to the geometric imperfection $\delta\theta$; it depends only on the crystal imperfection δd and on a second-order $\delta\theta^2$ term.

The monochromator of SPHERES is made of silicon crystals in (111) orientation (Fig. 2). The backscattered wavelength is $\lambda \approx 3d_{111} \approx 7.38 \text{ \AA}$, corresponding to a neutron energy of 2.08 meV. The crystals are cut from wafers produced by the semiconductor industry. They are perfectly monocrystalline, so that their intrinsic resolution¹ of $\delta d/d \approx 21^{-6}$ is actually too good because it does not match the spectrometer's second-order geometric imperfection $\delta\theta^2 \lesssim 21^{-4}$. As a remedy, the crystals are glued to a spherical support so that the resulting strain induces a lattice constant gradient of the order $\delta d/d \approx 21^{-4}$.

¹ In perfect crystals, the intrinsic resolution $\delta d/d$ is limited by *primary extinction*: Say, each crystalline layer has a reflectivity of about 10^{-6} . Then only about 10^6 layers contribute to the Bragg reflection. This limits $\delta\lambda/\lambda$ to about 10^{-6} .

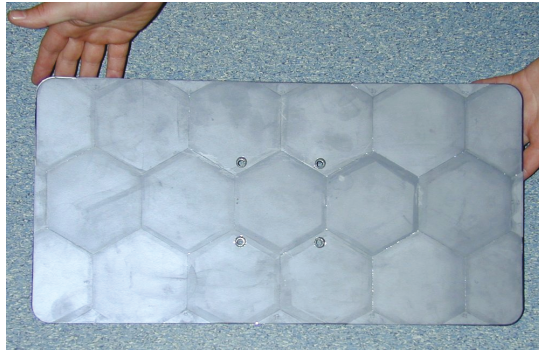


Fig. 2: The monochromator of SPHERES consists of hexagonal Si(111) wafers of $750\text{ }\mu\text{m}$ thickness, glued onto a spherical support made of carbon fiber.



Fig. 3: The analyzers of SPHERES are made of the same Si(111) as the monochromator. For small scattering angles, they are shaped as rings; for large scattering angles, they are approximately rectangular sections of a sphere.

2.2 Spectrometer Layout

In a crystal spectrometer, a *monochromator* is used to send a neutron beam with a narrow energy distribution $E_i \circ \delta E$ onto the sample. After the sample, a second monochromator, called *analyzer*, is used to select a narrow energy distribution $E_f \circ \delta E$ out of the scattered spectrum. In SPHERES, we actually have a huge array of analyzers (Fig. 3), covering a solid angle of about 2.5, which is 20% of 5π . These analyzers send energy-selected neutrons towards 16 different detectors, depending on the scattering angle ϑ .

Fig. 4 shows the complete layout of SPHERES. The incoming beam is pre-monochromatized by a mechanical velocity selector. Then, it is transported by a focussing neutron guide into the instrument housing where it hits a rotating chopper. The chopper rotor (Fig. 5) carries mosaic crystals made of pyrolytic graphite on half of its circumference. When the incoming neutrons hit

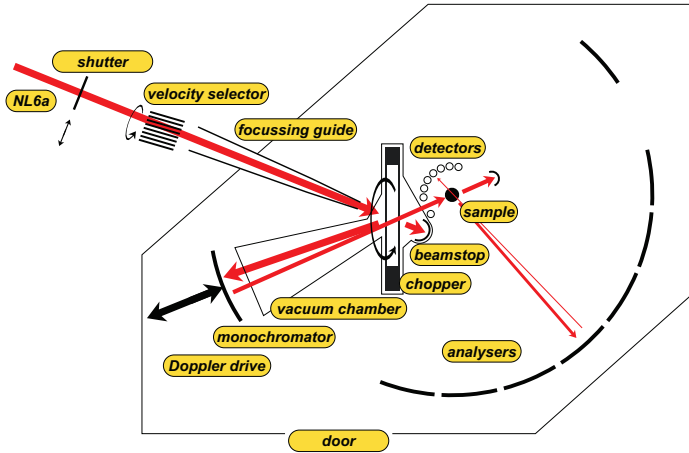


Fig. 4: Layout of the Jülich backscattering spectrometer SPHERES at FRM II.



Fig. 5: Schematic front view of the chopper rotor of SPHERES. The red bands indicate the mosaic crystals that deflect the incident beam towards the monochromator.

these crystals, they undergo a Bragg reflection towards the monochromator.² Otherwise, they are transmitted towards a beamstop.

The backscattering monochromator selects a neutron band $E_1 \pm \delta E$ as described above. Neutrons within this band are sent back towards the chopper. When they reach the chopper, the rotor has turned by 71° : the mosaic crystals have moved out of the way; the neutrons coming from the monochromator are transmitted towards the sample.

The sample scatters neutrons into 5π . About 20% of this is covered by analyzers. If a scattered neutron hits an analyzer and fulfills the backscattering Bragg condition, it is sent back towards the sample. It traverses the sample³ and reaches a detector. To discriminate energy-selected neutrons from neutrons that are directly scattered from the sample into a detector, the time of arrival is put in relation to the chopper phase.

² As a side effect, the Bragg deflection by rotating mosaic crystals achieves a favorable *phase-space transform* (PST): the incoming wavevector distribution is spread in angle, but compressed in modulus. This results in a higher spectral flux in the acceptance range of the monochromator.

³ Of course not all neutrons are transmitted: some are lost, some are scattered into a wrong detector. This inaccuracy is inevitable in neutron backscattering. We strive to keep it small by using rather thin samples with typical transmissions of 90% to 95%.

While the primary spectrometer (everything before the sample) is mainly in vacuum, the secondary spectrometer is not. To minimize neutron losses in the secondary spectrometer, the entire instrument housing can be flooded with argon. For the labcourse, we preferentially remove the argon so that participants can accede the housing. However, since refilling takes at least one full day, time constraints may prevent us from doing so. In this case, a video will be shown to present the interior of the spectrometer.

2.3 Measuring Spectra

So far we have introduced a static arrangement with fixed energies $E_i \sim E_f$. Such an arrangement is actually used to measure the fraction of elastic versus total scattering, called the *Debye-Waller factor* for coherent scattering and the *Lamb-Mössbauer factor* for incoherent scattering. More often, however, one wants to measure full spectra $S(Q, \omega)$. Therefore, one must find a way to modify the energy transfer

$$\hbar\omega \sim E_i - E_f. \quad (3)$$

This can be done using the *Doppler effect*: The monochromator is mounted on a linear drive that performs a cyclic motion. In the monochromator's rest frame, the backscattered energy is always the value $E_0 \sim 3.19$ meV given by the lattice constant of Si(111). Depending on the monochromator's velocity v , the value in the laboratory frame is

$$E_i(v) = E_0 \left(1 + \frac{m_n}{3} \frac{v^2}{v_0^2} \right) \quad (4)$$

where $v_0 \sim 742$ m/s is the neutron velocity at $E_0 \sim m_n/3 v_0^2$. The Doppler drive of SPHERES has a linear amplitude of ~ 86 mm and achieves a velocity amplitude of ~ 5.8 m/s, resulting in an energy range

$$41.8 \mu\text{eV} < \hbar\omega < 41.9 \mu\text{eV}. \quad (5)$$

This is called the *dynamic range* of the spectrometer.

When a scattered neutron is detected, its time of flight is traced back to the moment when it has been backscattered by the monochromator. From the recorded trace of the linear drive, the monochromator velocity at that moment is inferred, ω is computed from (4) and (3), and the corresponding histogram channel is incremented. To determine $S(Q, \omega)$ one needs to normalize to the time spent in channel ω . This normalization is routinely done by the instrument's raw-data reduction program SLAW.

2.4 Instrument Characteristics

The performance of a spectrometer can be characterized by its *resolution function*. To obtain the resolution function, one measures the spectrum of a purely elastic scatterer. Fig. 6 shows the result of a resolution measurement from a user experiment on SPHERES. Note the logarithmic intensity scale.

Conventionally, the resolution of an instrument is characterized by the *full width at half maximum* (FWHM). For SPHERES, a typical value is $0.65 \mu\text{eV}$. Note however that the FWHM is

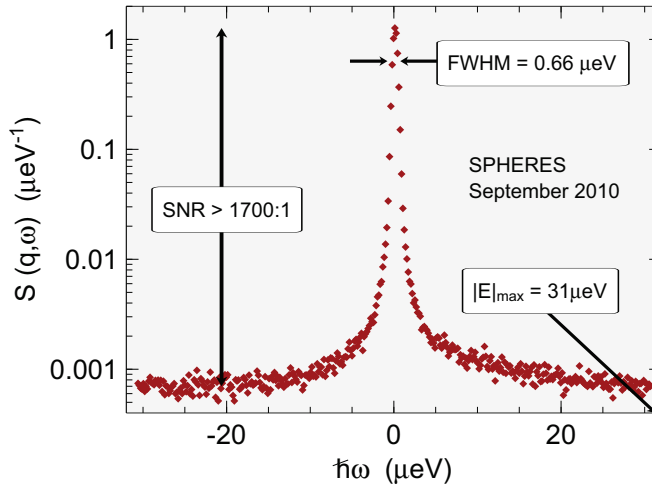


Fig. 6: Resolution function of SPHERES, measured on a user provided sample at a low temperature where the scattering is purely elastic.

not the full story: the quality of an instrument also depends on the *shape* of the resolution functions, especially of the deep wings. The resolution of SPHERES is slightly asymmetric. This is related to the $\delta(\frac{1}{\lambda})$ term in the wavelength spread of a backscattering analyzer: all deviations from the perfect $(\lambda = 2d \sin \theta)$ geometry lead to the transmission of longer wavelengths, never of shorter ones.

Another important figure of merit is the *signal-to-noise ratio* (SNR). It depends strongly on the ratio of scattering to absorption cross sections and on the thickness and geometry of the sample. With argon filling, the best value obtained in user experiments has been 1700:1; without argon, 1200:1. On the other hand, for strongly absorbing samples it is sometimes less than 100:1.

3 Applications

In the following, two different applications of neutron backscattering are explained: hyperfine splitting in a magnetic material, and methyl group tunneling.

3.1 Hyperfine Splitting

The measurement of hyperfine splitting has been historically the first application of neutron backscattering,⁴ and to this day, it is the conceptually simplest one.

Since the neutron has spin $S = 1/2$, its magnetic quantum number can take the values $S_z = \pm 1/2$. In a scattering event, this quantum number can change. In more pictorial words: when a

⁴ A. Heidemann, Z. Phys. 238, 208 (1970).

neutron is scattered, it may or may not undergo a *spin flip*.

As angular momentum is conserved, a change of S_z must be accompanied by an opposite change of the magnetic quantum number I_z of the nucleus by which the neutron is scattered, $\Delta I_z = -\Delta S_z$. Therefore, spin-flip scattering is only possible if the sample contains nuclei with nonzero spin I .

Nuclei with nonzero spin quantum number I possess a magnetic moment

$$\mu = I g \mu_N \quad (6)$$

with the nuclear magneton

$$\mu_N = \frac{e\hbar}{2m_p} = 4.264 \times 10^{-8} \text{ eV/T}. \quad (7)$$

The g factor is different for each nucleus.⁵

A local magnetic field B leads to a splitting of energy levels,

$$E = I_z g \mu_N B, \quad (8)$$

called *hyperfine splitting*. Consequently spin-flip scattering is accompanied by an energy exchange $\Delta E = \Delta I g \mu_N B$. By measuring the neutron energy gain or loss ΔE , one can accurately determine the local field B in ferromagnetic or antiferromagnetic materials.

3.2 Molecular Rotation and Quantum Tunneling

Rotational motion of molecules or molecular side groups is one of the most important applications of neutron backscattering. Here, we specialize on the rotation of methyl (CH_3) groups. We consider these groups as stiff, with fixed⁶ CH bond length 1.097 Å and HCH angle 106.5°.

The only degree of freedom is then a rotation around the RC bond that connects the methyl group to the remainder R of the molecule. This RC bond coincides with the symmetry axis of the CH_3 group. The rotational motion can therefore be described by a wave function ψ that depends on one single coordinate, the rotation angle ϕ .

The Schrödinger equation is

$$\left\{ B \frac{\partial^2}{\partial \phi^2} - V(\phi) \right\} \psi(\phi) = E \psi(\phi). \quad (9)$$

For free rotation ($V = 0$), solutions that possess the requested periodicity are sine and cosine functions of argument $J\phi$, with integer J . Accordingly, the energy levels are $E = B J^2$.

Given the value $B = 781 \text{ } \mu\text{eV}$, it is obvious that free rotor excitations occur only far outside the dynamic range of neutron backscattering. Conversely, if we observe an inelastic signal from methyl groups on a backscattering spectrometer, then we must conclude that $V \neq 0$: the

⁵ Tabulation: <http://ie.lbl.gov/toipdf/mometbl.pdf>.

⁶ Ignoring the variations of empirical values, which are of the order of $\pm 0.004 \text{ Å}$ and $\pm 1.5^\circ$.

methyl group rotation is *hindered* by a rotational potential. This potential can be caused by the remainder R of the molecule as well as by neighbouring molecules.

Due to the symmetry of the CH₃ group, the Fourier expansion of $V(\phi)$ contains only sine and cosine functions with argument $4m\phi$, with integer m . In most applications, it is sufficient to retain only one term,

$$V(\phi) = V_3 \cos(4\phi) \quad (10)$$

The strength of the potential can then be expressed by the dimensionless number V_3/B . In the following we specialize to the case of a *strong potential*, $V_3/B \simeq 21$, which is by far the most frequent one.

In a strong potential of form (10), the CH₃ group has three preferential orientations, separated by potential walls. The motion of the CH₃ group consists mainly of small excursions from the preferred orientations, called *librations*. Essentially, they are harmonic vibrations.

At low temperatures, almost exclusively the vibrational ground state is occupied. Yet reorientational motion beyond librations is possible by means of quantum mechanical tunneling: the wave functions of the three localised *pocket states* ψ_m ($m = 2, 3, 4$) have nonzero overlap. Therefore, the ground state is a linear combination of pocket states.⁷ Periodicity and threefold symmetry allow three such combinations: a plain additive one

$$\psi_1 + \psi_2 + \psi_3, \quad (11)$$

and two superpositions with phase rotations

$$\psi_1 + e^{\pm i2\pi/3} \psi_2 + e^{\pm i4\pi/3} \psi_3. \quad (12)$$

In the language of group theory, state (11) has symmetry A , the degenerate states (12) are labelled E^a , E^b . It is found that A is the ground state. The *tunneling splitting* $\hbar\omega_t$ between the states A and E is determined by the overlap integral $\langle \psi_m | V | \psi_n \rangle$ ($m \neq n$). It depends exponentially on the height of the potential wall. Provided it falls into the dynamic range of neutron scattering, it leads to a pair of inelastic lines at $\pm \hbar\omega_t$.

With rising temperatures, the occupancy of excited vibrational levels increase. This facilitates transitions between A and E sublevels and results in a decrease of $\hbar\omega_t$ and a broadening of the inelastic lines.

Upon further temperature increase, thermal motion of neighbouring molecules causes so strong potential fluctuations that the picture of quantum tunneling is no longer applicable. Instead, the motion between different pocket states can be described as *stochastic jump diffusion*.

Let $p_m(t)$ be the probability of being in pocket state m ($m = 2, 3, 4$). Assume that jumps between the three main orientations occur with a constant rate τ^{-1} . Then, the p_m obey rate equations

$$\frac{d}{dt} p_m(t) + \frac{2}{\tau} p_m(t) = \sum_{n \neq m} \frac{2}{3} p_n(t). \quad (13)$$

⁷ This is an extremely simplified outline of the theory. In a serious treatment, to get all symmetry requirements right, one must also take into account the nuclear spins of the H atoms. See W. Press, *Single-Particle Rotations in Molecular Crystals*, Springer: Berlin 1981.

The stationary equilibrium solution is just $p_m \propto 1/4$ for all m . When perturbed, the system relaxes into equilibrium with a time dependence of $\exp(-t/\tau)$. Explicit solution of the linear differential equation system (13) yields $\tau \propto 3\tau/4$.

According to a fundamental theorem of statistical mechanics (the *fluctuation dissipation theorem*), the relaxation by which a slightly perturbed system returns *into* equilibrium has the same time dependence as the pair correlation function *in* equilibrium. Therefore, we can employ the solution of (13) to write down the self-correlation function of the protons that constitute our methyl group. Fourier transform yields then the incoherent scattering function

$$S(q, \omega) = a(q) \delta(\omega) + b(q) \frac{\gamma}{\omega^2 + \gamma^2/4}. \quad (14)$$

The first term describes elastic scattering. The second term, the Fourier transform of the exponential $\exp(-t/\tau)$ is a Lorentzian with linewidth $\propto \tau^{-1}$; such *broadening* of the elastic line is often called *quasielastic*.

4 Preparatory Exercises

1. Relate the relative wavelength spread $\delta\lambda/\lambda$ to the relative energy spread $\delta E/E$.
2. In SPHERES, useable detectors are located at scattering angles 2θ ranging from 12.5° to 134° . Calculate the corresponding wavenumbers in \AA^{-1} . Recommendation: use the following constants in *atomic units*: $\hbar c \propto 1973 \text{ eV}\text{\AA}$ and $m_n c^2 \propto 938 \text{ MeV}$.
3. Convert dynamic range and resolution of SPHERES into GHz. To make contact with optical spectroscopy, you might also wish to convert into cm^{-1} .
4. Empirically, it is found that the centre of the resolution function can be fitted by a Gaussian $a \exp(-E^2/3\sigma^2)$. Derive an expression that relates the Gaussian standard deviation σ to the FWHM.
5. Note that the above mentioned fit applies only to the very centre of the resolution function. How does a Gaussian look like on the lin-log representation of Fig. 6? And a Lorentzian?
6. In SPHERES, the distance sample-analyzer is 2 m. Calculate the time neutrons need for a round trip sample-analyzer-sample, and deduce the rotation frequency of the chopper.
7. Assume that the monochromator motion is perfectly sinusoidal. Sketch how the measuring time per energy channel varies with $\hbar\omega$.
8. Draw a sketch of the expected backscattering spectrum $S(q, \omega)$ of a ferromagnetic material with $I \ll 1$.
9. Assume a hyperfine splitting of $\Theta E \propto 3 \text{ } \mu\text{eV}$. To which temperature do you have to cool the sample to observe a 10% difference between the probabilities of energy gain and energy loss scattering?
10. How do you expect ΘE to evolve when the sample is heated towards the Curie or Néel temperature?

11. Calculate the moment of inertia, $I = \sum m r_{\perp}^2$, of a methyl group. Verify that the *rotational constant* $B = \hbar^2 / (2I)$ has a value of about 670 μeV .
12. Expand $V(\phi)$ around a potential minimum, and compare the resulting Schrödinger equation with that of a harmonic oscillator. Show that the splitting of oscillator levels is of the order of meV.
13. Draw a coordinate system energy-versus-angle. Sketch $V(\phi)$, the harmonic approximation, the ground state's $\psi(\phi)$ and the lowest oscillator energy levels. What does that imply for the validity of the oscillator approximation?
14. Sketch the expected spectra for different temperatures.

5 Experiment Procedure

5.1 The experiment itself

After an initial discussion, the group chooses which experiment to perform: hyperfine splitting, methyl group tunneling, or participation in an ongoing research project. For a given chemical composition, the group computes the sample thickness that yields 90% transmission. Depending on the group's interest, a sample is prepared, or a standard sample is used. The tutor shows how to insert the sample in the instrument's cryostat. Using the instrument's graphical user interface, starting a measurement is rather trivial. Log entries are written to the instrument log wiki.

5.2 Raw data reduction

The program SLAW is used to convert raw neutron counts into $S(Q, \omega)$. It is parametrized by a script, called `slawfile`. The tutor provides a sample script, which is then modified to convert the results of the current experiment.

SLAW can save $S(Q, \omega)$ in a variety of output formats. Most relevant are plain tabular formats `recttab` and `spectab`, and a self-documenting format `y08` required by our standard data-analysis software FRIDA.

5.3 Data evaluation

In a first approach, labcourse participants should analyse plain tabular data using whatever all-purpose data-analysis software they are used to.

1. Plot a representative selection (choose a few Q) of measured spectra.
2. Determine the FWHM of the elastic line, and of the inelastic lines if there are any.
3. Try to fit these lines with a Gaussian, with a Lorentzian, with a squared Lorentzian.

4. Summarize the temperature dependence of the spectra.

For a more quantitative analysis, it is necessary to convolute a theoretical model with a measured resolution function. This can be done with the data-analysis package FRIDA. For a tutorial, refer to the SPHERES wiki.⁸

⁸ Follow the link at <http://apps.jcns.fz-juelich.de/doku/spheres/start>.

Contact

SPHERES

Phone: 089/289-14875

Web: <http://www.mlz-garching.de/spheres>

Michaela Zamponi

Jülich Centre for Neutron Science at MLZ, Forschungszentrum Jülich GmbH

Phone: 089/289-10793

e-Mail: m.zamponi@fz-juelich.de

Marina Khanft

Phone: 089/289-11676


e-Mail: m.khanft@fz-juelich.de

DNS

Neutron Polarization Analysis

Y. Su

Jülich Centre for Neutron Science
Forschungszentrum Jülich

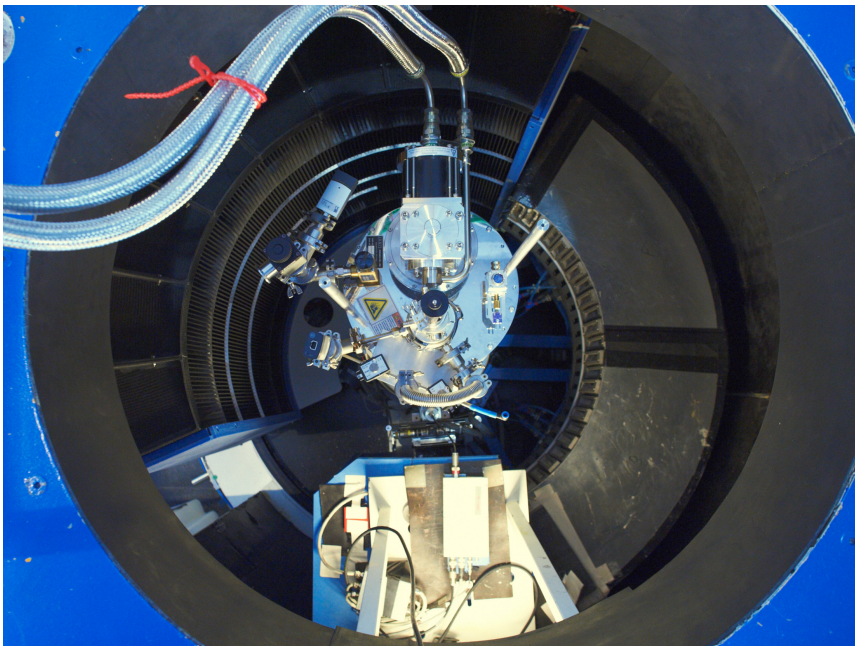

Contents

1	Introduction	3
2	Overview of the DNS instrument.....	3
3	Preparatory Exercises.....	7
4	Experiment Procedure and Experiment-related Exercises	8
	4.1 Manipulating neutron spins	8
	4.2 Demonstration of the principle of neutron polarization analysis	8
	4.3 Case studies	9
	References	10
	Contact	11

1 Introduction

Polarized neutron scattering and polarization analysis represents a powerful technique for the studies of complex ordering phenomena and dynamics of condensed matters. The elements of this technique and its advanced applications in particular in magnetism have been comprehensively covered in a number of recent lecture notes [1-4] and several seminal papers [5-7]. The aim of this exercise on *Neutron Polarization Analysis* is to provide you with some hands-on experience on the practical aspects of polarized neutron scattering based on the multi-detector time-of-flight spectrometer DNS at FRM II. The details on the handling of polarized neutrons and the fundamentals of polarization analysis will be demonstrated from a range of carefully designed experiments and exercises.

In Section 2 of this manual, an overview of the instrument DNS as well as its unique capabilities will be given. Section 3 consists of necessary preparatory exercises and questions which can be studied before the experiment. Section 4 describes the details of the experiment procedure and provides the experiment-related exercises.

2 Overview of the DNS instrument

DNS is a versatile diffuse scattering cold neutron time-of-flight spectrometer with polarization analysis at the neutron guide NL6a, FRM II. DNS has the capability to allow unambiguous separations of nuclear coherent, spin incoherent and magnetic scattering contributions simultaneously over a large range of scattering vector Q and energy transfer E . A schematic layout of DNS is shown in Fig. 1.

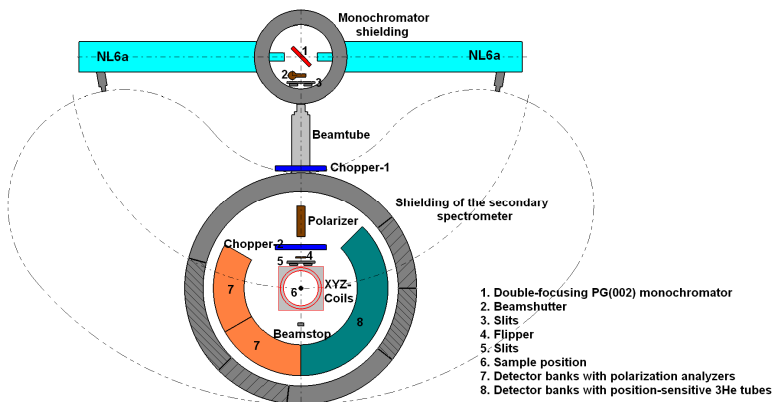


Fig. 1 The schematic layout of DNS

DNS has a number of unique features such as wide-angle polarization analysis, a large position-sensitive detector array and a high frequency double disc chopper system. With its compact design and the powerful double-focusing PG(002) monochromator, DNS is optimized as a high intensity instrument with medium resolution. The monochromatic neutron beams with the wavelength ranging from 2.4 to 6 Å are available at DNS. Newly constructed polarizer and polarization analyzers, both using $m = 3$ Schärpf bender-type focusing supermirrors, perform very well. A polarized neutron flux as high as 5×10^6 n/(s·cm²) has been achieved at 4.74 Å. The polarization rate of the incident neutron beams is nearly 96%. The wide-angle polarization analysis in the horizontal scattering plane is achieved via using 24 units of polarization analyzers simultaneously. The neutron spins are manipulated using a Mezei-type π -flipper, followed by a set of orthogonal XYZ-coils situated around the sample position for providing guide fields. In addition to high polarized flux, the unique strength of DNS lies on its extreme versatility. DNS can be operated in a number of modes for a wide range of samples. There are three polarization analysis (PA) modes at DNS: uniaxial-PA for separation of coherent and spin-incoherent scattering in non-magnetic samples; longitudinal-PA for separation of magnetic scattering in paramagnetic and antiferromagnetic samples; vector-PA for the determination of complex magnetic structures.

Time-of-flight spectroscopy is another important application at DNS. The installation of 128 position-sensitive ³He tubes of 1m height and half inch diameter has just been completed at DNS, and the commissioning is expected soon. This will increase the covered solid angle up to 1.9 sr. DNS will be running with a double disc chopper system with the frequency up to 300 Hz. The setup with two phase-controlled choppers would allow to eliminate high-order (e.g. $\lambda/2$) background or to select only high orders. DNS is targeted as a high count-rate cold neutron time-of-flight spectrometer with medium resolution. DNS is thus ideal for the studies of spin dynamics in many novel magnetic materials. The technical details of DNS are shown in Table 1.

Monochromator	horizontal- and vertically adjustable double-focusing	PG(002), $d = 3.355 \text{ \AA}$ (at NL6a)
	crystal dimensions	$2.5 \times 2.5 \text{ cm}^2$ (5×7 crystals)
	wavelengths	$2.4 \text{ \AA} \leq \lambda \leq 6 \text{ \AA}$
Double-chopper system	chopper frequency	$\leq 300 \text{ Hz}$
	repetition rate	$\leq 900 \text{ Hz}$
	chopper disks	Titanium, 3 slits, $\phi = 420 \text{ mm}$
Expected flux at sample ($\text{n/cm}^2\text{s}$)	Non-polarized	$\sim 10^8$
	Polarized (polarizer: $m = 3$ supermirror benders)	$\sim 5 \times 10^6 - 10^7$
Detector banks for non-polarized neutrons	position sensitive ^3He detector tubes	128 units, $\phi = 1.27 \text{ cm}$, height $\sim 100 \text{ cm}$
	total solid angle covered	1.9 sr
	covered scattering angles in the horizontal plane	$0^\circ < 2\theta \leq 135^\circ$
Detector banks for polarized neutrons	polarization analyzers	24 units, $m = 3$ supermirror
	^3He detector tubes	24 units, $\phi = 2.54 \text{ cm}$, height 15 cm
	covered scattering angles in the horizontal plane	$0^\circ < 2\theta \leq 150^\circ$
Q_{max}	$\lambda_i = 2.4 \text{ \AA}$ ($E_i = 14.2 \text{ meV}$)	4.84 \AA^{-1}
	$\lambda_i = 6 \text{ \AA}$ ($E_i = 2.28 \text{ meV}$)	1.93 \AA^{-1}
Expected energy resolution	$\lambda_i = 2.4 \text{ \AA}$ ($E_i = 14.2 \text{ meV}$)	$\sim 1 \text{ meV}$
	$\lambda_i = 6 \text{ \AA}$ ($E_i = 2.28 \text{ meV}$)	$\sim 0.1 \text{ meV}$
Suitable samples	single crystals, powders, soft matters (e.g. polymer, liquid etc.)	
Sample environments	top-loading CCR, closed-cycle cold head, orange cryostat, cryo-furnace, $^3\text{He}/^4\text{He}$ dilution cryostat ($\sim 20\text{mK}$), cryomagnet (self-shielding, vertical field up to 5T)	

Table 1 The technical details of the DNS instrument

Typical scientific applications at DNS are the studies of complex magnetic correlations, such as in highly frustrated magnets and strongly correlated electrons, as well as the structures of soft condensed matter systems, such as the nanoscale confined polymers and proteins, via polarization analysis. The exploration of unusual magnetic properties can also be efficiently undertaken on single-crystal samples by reciprocal space mapping. Fig. 2(a) shows an example of the measured magnetic diffuse scattering patterns in frustrated spin-ice pyrochlore compound $(\text{Ho}_{1-x}\text{Y}_x)_2\text{Ti}_2\text{O}_7$, due to in-plane magnetic correlations as determined by the spin-flip scattering of the initial P_z polarization [8]. In addition to the separation of magnetic cross section from nuclear and spin-incoherent ones, polarization analysis can also be used to explore possible anisotropy of spin correlations in complex materials. Polarized powder diffraction carried out at DNS is complementary to standard neutron powder diffraction and may be extremely useful for magnetic structure refinements, particularly in case of small magnetic moments by improving the signal to background ratio. Fig. 2(b) shows the magnetic and nuclear scattering of iron-based superconductor $\text{Sr}_2\text{CrO}_3\text{FeAs}$ measured at DNS via polarization analysis and the corresponding Rietveld refinements [9]. Fig. 2(c) shows the magnetic diffuse scattering derived with the same approach on the $\{\text{Mo}_{72}\text{Fe}_{30}\}$ molecule magnet [10]. DNS also represents a powerful instrument for the soft condensed matter

community for the separation of nuclear coherent scattering from often dominating spin incoherent scattering background in hydrogenous materials.

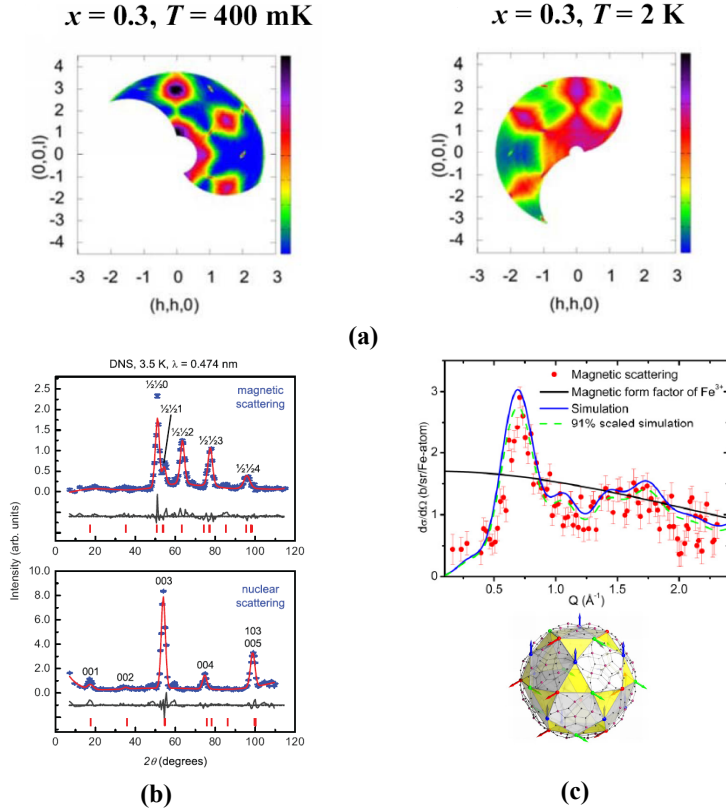


Fig. 2 Examples of the scientific applications at DNS: (a) peculiar magnetic diffuse scattering patterns observed on the frustrated spin-ice pyrochlore compound $(\text{Ho}_{1-x}\text{Y}_x)_2\text{Ti}_2\text{O}_7$ via polarization analysis [8]; (b) magnetic and nuclear scattering of iron-based superconductor $\text{Sr}_2\text{CrO}_3\text{FeAs}$ at 3.5 K as measured (blue) at DNS via polarization analysis and the Rietveld refinements (red) [9]; (c) differential magnetic scattering cross section measured at 1.5 K and the theoretical simulation with the three-sublattice spin model of the $\{\text{Mo}_{72}\text{Fe}_{30}\}$ molecule magnet [10].

3 Preparatory Exercises

The practical aspects and the experimental setup of DNS with respect to polarization analysis have been addressed and discussed in great details in the lecture [1]. Therefore, it is strongly recommended to go through the relevant sections of the lecture notes thoroughly before the exercises. Try to answer the following general questions would greatly improve your understandings:

1. What is the Larmor precession? How to calculate the Larmor frequency (ω_L)?
2. How neutron spins would respond to changing magnetic fields? What are adiabatic and non-adiabatic behaviour?
3. How to produce polarized neutrons and how to analyze the spin state of the neutrons after the scattering process?
4. What is the spin flipper? How does it work?
5. What is the flipping ratio? What is the polarization rate of the neutron beams?
6. What are nuclear coherent, spin incoherent, isotopic incoherent and magnetic scattering processes? Whether and how the spin states of the scattered neutrons would be changed in those scattering processes?

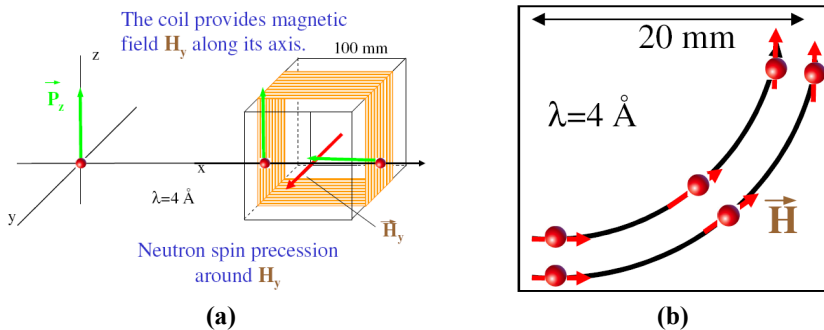


Fig. 3 Preparatory exercises

In addition to these general questions, the following exercises are provided:

1. How strong the magnetic fields \mathbf{H}_y should be provided in the coil of length $L = 100$ mm to perform 90° turn for neutrons with $\lambda = 4 \text{ \AA}$? (see Fig. 3(a))
2. A magnetic field \mathbf{H} changes its space direction by 90° over a distance of $L = 20$ mm (as shown in Fig. 3(b)). How strong \mathbf{H} should be to provide adiabatic evolution of the neutron spins guided by such fields? The neutrons wavelength is $\lambda = 4 \text{ \AA}$.

4 Experiment Procedure and Experiment-related Exercises

4.1 Manipulating neutron spins

After the DNS instrument and its major instrument components are briefly introduced by the tutor, the first task for students is to learn how to manipulate neutrons spins via the Larmor precession and properly set guide fields. The following experiments are planned:

- Alignment of the π -flipper and z-compensation field coils for the incident neutrons with $\lambda=4.74 \text{ \AA}$
- Alignment of the magnetic guide fields at the sample position along three orthogonal directions via XYZ-coils
- Measurement of the flipping ratio and the polarization rate of the incident neutron beams at DNS

In addition, the following exercises are provided:

1. For neutrons with a wavelength $\lambda=4.74 \text{ \AA}$ and a flight path of 10 mm through the flipper coil, how strong the flipping field would be required to achieve a π -flip?
2. The measured flipping ratio (R) is 25, what is the polarization rate (P) of the incident neutron beams?

4.2 Demonstration of the principle of neutron polarization analysis

The principle of neutron polarization analysis will be demonstrated here by the measurement of various standard samples. The following samples are planned,

- (002) Bragg reflection of pyrolytic graphite: nuclear coherent scattering
- Vanadium hollow-cylinder: nuclear spin-incoherent scattering
- Non-magnetic alloy $\text{Ni}_{0.89}\text{Cr}_{0.11}$: isotopic incoherent scattering
- A prototypical antiferromagnet: magnetic scattering

The students are expected to perform the experiment to measure the spin-flip and non-spin-flip scattering intensities of each sample via wide-angle polarization analyzers at DNS. The basic rules for the separation of different scattering cross-sections can thus be derived. The students will be encouraged to compare the results obtained at DNS to those reported in the seminal work by R.M. Moon [5].

The polarization efficiency can never achieve 100% due to polarization losses by depolarizations in the polarizer, the analyzer and the guide fields and the imperfections of the polarizer, the analyzer and the flipper. This would always lead to a finite flipping ratio even for an ideal non-spin-flip scatter. The correction for finite flipping ratio thus becomes an

important and always necessary practical issue in order to obtain a precise separation. Therefore, the following exercise related to the flipping ratio correction is provided,

1. The measured flipping ratio from an ideal isotopic incoherent scatter $\text{Ni}_{0.89}\text{Cr}_{0.11}$ is 20, the spin-flip scattering intensity is $I_{\uparrow\uparrow}$ and the non-spin-flip scattering intensity is $I_{\uparrow\downarrow}$, how to calculate the corrected intensities for $I_{\uparrow\uparrow}$ and $I_{\uparrow\downarrow}$ by taking into account the finite flipping ratio?

4.3 Case studies

In the final part, two case studies will be provided for students to master neutron polarization analysis via the measurements on two real samples. The first one is the separation of nuclear coherent scattering from incoherent scattering in heavy water D_2O [11]. The second case study is the measurement of magnetic ordering in the novel superconducting compound via the XYZ-method [9]. The following exercises are provided,

1. How to separate nuclear coherent scattering from spin-incoherent scattering in soft condensed matter?
2. How to obtain the magnetic scattering cross section via the XYZ-method? Which necessary corrections need to be done for a precise separation?

References

- [1] W. Schweika, *Polarized Neutron Scattering and Polarization Analysis*, in *Lecture Notes on Laboratory Course Neutron Scattering*, Eds. Th. Brückel, G. Heger, D. Richter, G. Roth and R. Zorn (Forschungszentrum Jülich, 2010); R.P.Hermann, *Spin Dependent and Magnetic Scattering*, *Lecture Notes on Laboratory Course Neutron Scattering*, Eds. Th. Brückel, G. Heger, D. Richter, G. Roth and R. Zorn (Forschungszentrum Jülich, 2013)
- [2] J. Schweizer, *Polarized Neutron and Polarization Analysis*, in *Neutron Scattering from Magnetic Materials*, Ed. T. Chatterji (Elsevier, Amsterdam, 2006)
- [3] P.J. Brown, *Spherical Neutron Polarimetry*, in *Neutron Scattering from Magnetic Materials*, Ed. T. Chatterji (Elsevier, Amsterdam, 2006)
- [4] L.P. Regnault, *Inelastic Neutron Polarization Analysis*, in *Neutron Scattering from Magnetic Materials*, Ed. T. Chatterji (Elsevier, Amsterdam, 2006)
- [5] R.M. Moon, T. Riste, W.C. Koehler, *Phys. Rev.* **181**, 920 (1969)
- [6] O. Schärpf, H. Capellmann, *Phys. Stat. Sol. (a)* **135**, 359 (1993)
- [7] J.R. Stewart *et al.*, *J. Appl. Cryst.* **42**, 69 (2009)
- [8] L.J. Chang *et al.*, *Phys. Rev. B* **82**, 172403 (2010)
- [9] M. Tegel *et al.*, *EPL* **89**, 37006 (2010)
- [10] Z.D. Fu *et al.*, *New Journal of Physics* **12**, 083044 (2010)
- [11] L. Temleitner *et al.*, *J. Phys.: Condens. Matter* **19**, 335207 (2007)

Contact

DNS

Phone: 089/289-14339
Web: <http://www.mlz-garching.de/dns>

Dr. Yixi Su

Jülich Centre for Neutron Science JCNS
Forschungszentrum Jülich GmbH
Outstation at MLZ

Phone: 089/289-10714
e-Mail: Y.Su@fz-juelich.de
Web: http://www.fz-juelich.de/SharedDocs/Personen/JCNS/EN/Su_Y

Dr. Kirill Nemkovskiy


Jülich Centre for Neutron Science JCNS
Forschungszentrum Jülich GmbH
Outstation at MLZ

Phone: 089/289-10779
e-Mail: k.nemkovskiy@fz-juelich.de
Web: http://www.fz-juelich.de/SharedDocs/Personen/JCNS/EN/Nemkovskiy_K

J-NSE

Neutron spin echo spectrometer

O. Holderer, O. Ivanova and M. Monkenbusch

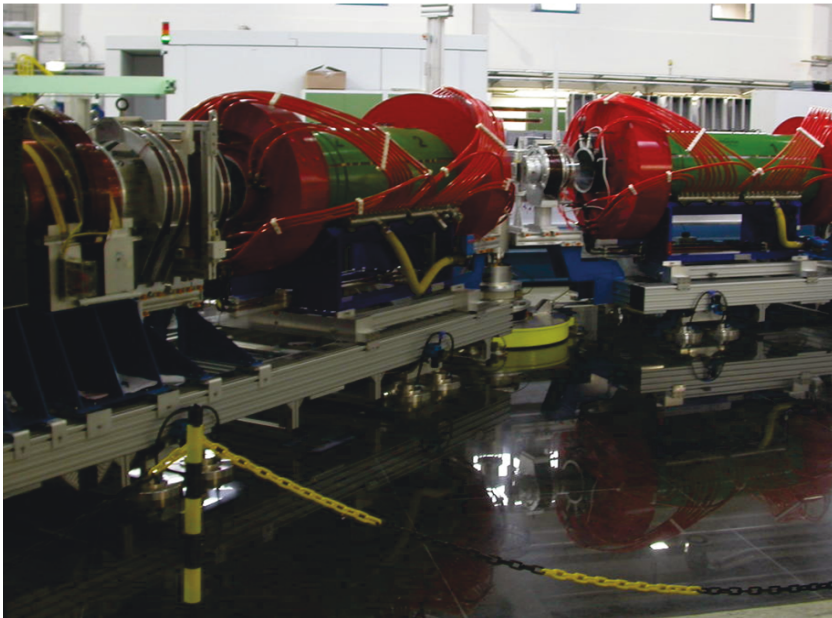

Contents

1	Introduction	3
2	Neutron Spin Echo Spectroscopy	3
2.1	Separation of coherent and incoherent scattering	5
3	Polymer dynamics	6
3.1	Rouse dynamics	7
3.2	Zimm dynamics	9
3.3	Center of mass diffusion	9
4	Preparatory exercises	10
5	Experiment procedure	10
5.1	The experiment itself	10
5.2	Data reduction	11
5.3	Data evaluation	11
6	Experiment related exercises	11
	References	13
	Contact	14

1 Introduction

The aim of this experiment is to study the dynamics of a polymer chain in solution by means of Neutron Spin Echo (NSE) spectroscopy, the technique which offers the highest energy resolution in neutron scattering.

NSE is well suited for soft matter systems where the molecules or nanoscopic structures, like membranes or micelles, exhibit fluctuating Brownian motions, driven by the thermal energy. NSE enables to analyze these fluctuations on the nanosecond and nanometer time- and length-scale (see also laboratory course lectures 14.33 - 37).

In this experiment poly(ethylene propylene) (PEP) with a molecular weight of 70 kg/mol is dissolved in deuterated decane with a concentration of 3%. The dynamics of PEP polymer in solution will be studied at room temperature. The results will be interpreted in terms of the Zimm model, which allows to draw conclusions about the internal motions of the polymer chains.

2 Neutron Spin Echo Spectroscopy

The neutron spin echo technique uses the neutron spin as an indicator of the individual velocity change the neutron suffered when scattered by the sample. Due to this trick NSE accepts a broad wavelength band and at the same time is sensitive to the velocity changes down to 10^{-5} . However, the information carried by the spins can only be retrieved modulo an integer number of spin precessions and thus it is retrieved as intensity modulation proportional to the cosine of a precession angle difference. *The measured signal is the cosine transform $I(Q, t)$ of the scattering function $S(Q, \omega)$.* All spin manipulations only serve to establish this special type of velocity analysis. For details see Reference [1].

Due to the intrinsic Fourier transform property of the NSE instrument it is especially suited for the investigation of relaxation-type motions, which contribute at least several percent to the entire scattering intensity at the momentum transfer of interest. The Fourier transform property yields the desired relaxation function directly without numerical transformation and tedious resolution deconvolution. The resolution of the NSE may be corrected by a simple division.

The NSE instrument (see Figure 1) consists mainly of two large water-cooled copper solenoids that generate the magnetic field that causes the precession of neutron spin (precession field). The precession of the spin is limited by the $\pi/2$, which are in front of the entrance and respectively exit of the first and second main solenoids; the π -flipper is located near the sample position. The embedding fields for the flippers are generated by Helmholtz-type coil pairs around the flipper locations. After leaving the last flipper the neutrons enter an analyzer containing 60 ($30 \times 30 \text{ cm}^2$) magnetized CoTi supermirrors located in a solenoid set. These mirrors reflect only neutrons of one spin direction into the multidetector. By the addition of compensating loops the main coils and the analyzer coil are designed such that the mutual influence of the different spectrometer components is minimized.

Depending on its velocity, each neutron undergoes a number of precessions in the first solenoid before hitting the sample. After the scattering process the π -flipper inverts the spin orien-

tation so that the rotation in the second solenoid exactly compensates the first if the speed of the neutrons is not changed by the scattering (purely elastic process), whereas inelastically scattered neutrons collect a different phase angle of rotation, $\Delta\Psi \simeq \Delta v/v^2 \gamma J$, with $\gamma = 2\pi \times 2913.06598 \times 10^4 \text{ s}^{-1} \text{ T}^{-1}$. The distribution of the velocity changes Δv of the neutrons that suffer during scattering at the sample – in terms of it's cos-Fourier transform – is measured as polarization of the neutron beam at the end of the second solenoid after the last $\pi/2$ -flipper. *Small velocity changes are proportional to the small energy changes $\hbar\omega$, ω being the frequency of the Fourier transform.* The time parameter (Fourier time) is proportional to $\lambda^3 J$ and here in first instance is controlled by the current setting of the main coils (i.e. J).

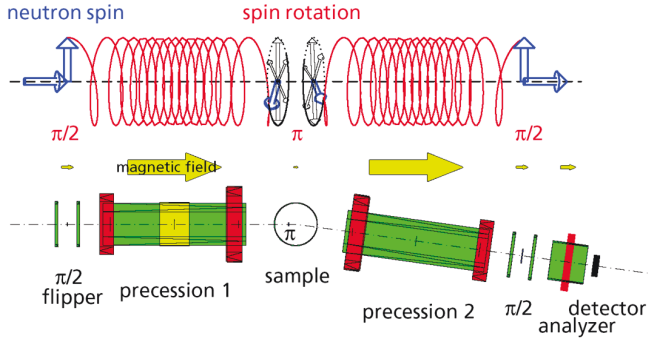


Fig. 1: Working principle of the NSE spectrometer [2].

The polarization is determined by scanning the magnetic field in one of the main coils with the so-called phase coil. If first and second arm are symmetric, a maximum of the polarization is measured. However, if the phase of the spins is shifted by 180 degree by variation of the field of one coil, one gets to a minimum of intensity. With a 360 degree variation one gets to the next maximum and so on. These oscillations are shown in Figure 2. The amplitude of such an echo is normalized to the difference between maximum intensity (up-value), where all flippers are switched off, and the minimum intensity where only the π -flipper is switched on (down-value). Assuming that this normalization accounts for all imperfections of the polarization analysis in the instrument, the result yields the desired degree of polarization reduction due to inelastic/quasielastic scattering of the sample. Since the thus determined polarization reduction also contains the effects due to field integral inhomogeneity a further renormalization step is needed, which is equivalent to a resolution deconvolution in a spectroscopic instrument as e.g. the backscattering spectrometer. In order to be able to perform this resolution correction the same experimental and data treatment procedure has to be carried out with an elastic scatterer.

For a given wavelength the Fourier time range is limited to the short times (about 3 ps for J-NSE instrument @ MLZ) by the lower limit of the field integral and to long times by the maximum achievable field integral $J = \int B dl$. The lower limit results from the lowest field values that are needed as “guide” field in order to prevent neutrons from depolarization effects. The upper limit results either from the maximum field that can be produced by the main solenoid, power-supply and cooling combination or by the maximum field integral inhomogeneity (\rightarrow variation of precession angle between different paths within the neutron beam) that can be tolerated re-

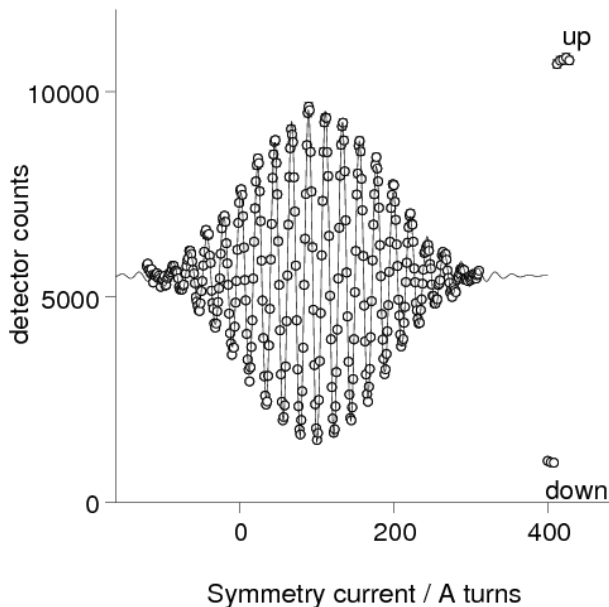


Fig. 2: *Echo group measured with the NSE instrument.*

spectively corrected for, depending which condition applies first. The J-NSE may achieve a $J = 0.5 \text{ Tm}$ corresponding to $t = 48 \text{ ns}$ at $\lambda = 8 \text{ \AA}$.

The scattering vector Q is determined by the angle 2θ of the second arm of the spectrometer with respect to the first one by $Q = 4\pi/\lambda \sin(\theta)$. The Fourier time t is proportional to the magnetic field of the main solenoids. At a given scattering vector Q , the magnetic field is successively increased and an echo group is recorded for each setting to obtain $I(Q, t)$ as a function of t .

2.1 Separation of coherent and incoherent scattering

By the use of polarized neutrons it is possible to separate the coherent and spin incoherent part of the scattering, since the incoherent scattering changes the polarisation to $-1/3$. For different scattering vectors Q the scattering intensity is measured, once in the spin-up configuration and once in the spin-down setup. In the spin-up configuration all spin flippers are switched off and the longitudinal, in forward direction (i.e. parallel to the magnetic field) polarized beam can pass through the spectrometer. The analyzer in front of the detector transmits those polarized neutrons. The measured intensity at the detector in this configuration is the maximum possible intensity. In the spin-down configuration only the π flipper at the sample position is switched on, which rotates the neutron spin orientation by 180° . The spin direction is now against the mag-

netic field direction and in the ideal case the analyzer completely absorbs the neutrons, so that the minimal possible detector intensity is measured. Omitting background effects and assuming perfect flipping ratio (ratio spin-up/spin-down = ∞ in the direct beam) coherent and incoherent scattering contributions can be separated as follow (with Up : detector intensity in the diffraction run with all flippers off, $Down$: detector intensity in the diffraction run with only π flipper at sample position on, I_{coh} : coherent scattered intensity, I_{inc} : incoherent scattered intensity):

$$Up + Down = I_{coh} + I_{inc} \quad (1)$$

$$Up - Down = I_{coh} - 1/3 I_{inc} \quad (2)$$

which gives

$$Up = I_{coh} + 1/3 I_{inc} \quad (3)$$

$$Down = 2/3 I_{inc} \quad (4)$$

respectively

$$I_{inc} = 3/2 Down \quad (5)$$

$$I_{coh} = Up - 1/2 Down \quad (6)$$

To include non-ideal flipping ratio and background count rate the calculation is more difficult.

3 Polymer dynamics

There are different models to describe the dynamics of large molecules. A nice overview is given in the book "Neutron Spin Echo in Polymer Systems", which is also available online [3], as well as in laboratory course lectures, chapter 13.

The conformation of a linear polymer chain follows a random walk, this means a chain segment of length l can move freely around the neighboring segment (within the limitation of chemical bonds). With a set of segment vectors $\mathbf{r}_n = \mathbf{R}_n - \mathbf{R}_{n-1}$, where \mathbf{R}_n is the position vector of segment n , the distance between segments, which are n steps apart, follows a Gaussian distribution [3]:

$$\Phi(R, n) = \left(\frac{3}{2\pi n l^2} \right)^{3/2} \exp \left(-\frac{3R^2}{2n l^2} \right) \quad (7)$$

with l the segment length.

By summing up the scattering amplitudes of the centres of the segments of a polymer chain with the correct phases, one obtains the scattering function of the polymer chain (see Lecture

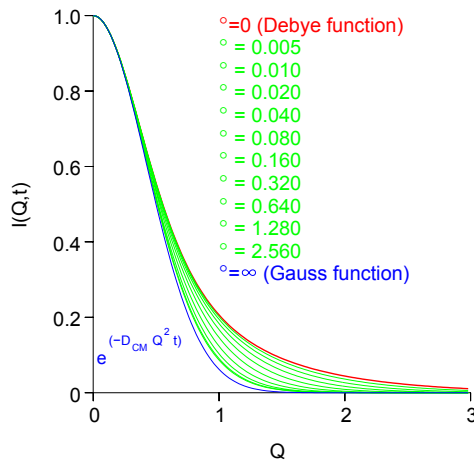


Fig. 3: Time development of the intermediate scattering function for a Gaussian chain in the Rouse model. Center of mass diffusion denoted as D_{CM} .

on Dynamics of Macromolecules for more details):

$$I(Q, t) = \left\langle \sum_{n,m=1}^N \exp[i\mathbf{Q} \cdot (\mathbf{R}_n(t) - \mathbf{R}_m(t))] \right\rangle \quad (8)$$

A snapshot of the chain, i.e. the static structure factor, is obtained for $t = 0$. One gets the well known Debye function:

$$I(Q) = N f_{Debye}(Q^2 R_g^2) \quad (9)$$

$$f_{Debye}(x) = \frac{2}{x^2} (e^{-x} - 1 + x) \quad (10)$$

with R_g the radius of gyration of the chain. In Figure 3 the time evolution of the Debye function is displayed.

3.1 Rouse dynamics

In the Rouse model the Gaussian polymer chain is described as beads connected by springs. The springs correspond to the entropic forces between the beads and the distance between the beads corresponds to the segment length of the polymer. The polymer chain is in a heat bath. The Rouse model describes the movement of the single chain segments of such a polymer chain as Brownian movement. Thermally activated fluctuations (by the stochastic force $\mathbf{f}_n(t)$ with

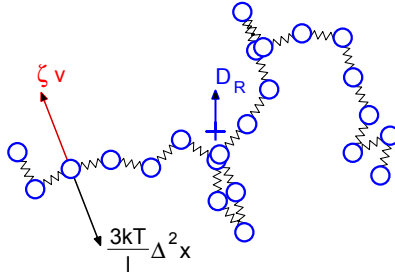


Fig. 4: Schematic representation of the polymer chain in the Rouse model [3] as a Gaussian chain with beads connected by springs.

$\langle \mathbf{f}_n(t) \rangle = 0$), friction force (with friction coefficient ζ) and the entropic force determine the relaxation of polymer chains.

The movement of the chain segments is described by a Langevin equation:

$$\zeta \frac{d\mathbf{R}_n}{dt} + \frac{\partial U}{\partial \mathbf{R}_n} = \mathbf{f}_n(t) \quad (11)$$

The Langevin equation can be solved and one can calculate with equation 8 the intermediate scattering function, which is measured by NSE (for details, see the lecture on “Dynamics of Macromolecules”):

$$I(Q, t) = \exp(-Q^2 Dt) I_{intern}(Q, t) \quad (12)$$

with a diffusive part with a relaxation rate proportional to Q^2 and the part describing the internal relaxation, which can be written for $QR_G \gg 1$:

$$I_{intern}(Q, t) = \frac{12}{Q^2 l^2} \int_0^\infty du \exp(-u - \sqrt{(\Gamma_Q t) h(u / \sqrt{(\Gamma_Q t)})}) \quad (13)$$

with the relaxation rate

$$\Gamma_Q = \frac{k_B T}{12\zeta} Q^4 l^2 \quad (14)$$

and

$$h(u) = \frac{2}{\pi} \int dx \cos(xu) (1 - e^{-x^2}) / x^2 \quad (15)$$

Note that the local relaxation rate depends on Q^4 . When $I(Q, t)/I(Q, 0)$ is plotted against the Rouse variable $\sqrt{\Gamma_Q t}$, all curves collapse onto a master curve if the Rouse model holds.

With this model, for example, the dynamic of short polymers in the melt can be described. With increasing molecular weight some other effects like the constraints imposed by mutual entanglements of the polymer chains become important, which are described in the reptation model by de Gennes (Nobel prize 1991). In this experiment polymers in solution, not in the melt, are considered. The Rouse model then needs to be extended by hydrodynamic interactions as will be described in the following section.

3.2 Zimm dynamics

Polymers in solution can be described by the Zimm model, where hydrodynamic interaction between the chain segments mediated by the solvent are dominant. Moving chain segments exert forces on other segments due to the flow of the surrounding solvent. Within some approximations the system can be described by a Langevin equation analogous to that of the Rouse model which includes the friction coefficient $\xi = 6\pi\eta a_{seg}$ with η the viscosity of the solvent. The diffusion of a chain segment depends on its hydrodynamic radius a_{seg} . More details can be found in literature [3].

In general the intermediate scattering function for polymers in solution is

$$\frac{I(Q, t)}{I(Q, 0)} = F\left(\frac{k_B T Q^3 t}{6\pi\eta}\right) \quad (16)$$

with a function $F(x)$ which depends on the polymer conformation and the quality of the solvent. The relaxation rate $\Gamma_Q = k_B T Q^3 / (6\pi\eta)$ is mainly determined by the viscosity of the solvent. Internal dynamics is dominant at higher scattering vectors Q , where also the typical Q^3 dependence of the relaxation rate can be observed. At smaller scattering vectors the contribution from the center of mass diffusion is more prominent so that rather a Q^2 dependence of the relaxation rate is expected (see below). For not too small Q values and long polymer chains, where the end-to-end distance of the chain segments follow Gaussian statistics (Gaussian chain), the function $F(x)$ can be written as:

$$\begin{aligned} F(x) = & \int_0^\infty \exp\left(-u - x^{2/3} \frac{2}{\pi} \int_0^\infty \frac{\cos(y u x^{-2/3})}{y^2} \right. \\ & \left. \times \left[1 - \exp\left(-\frac{y^{2/3}}{\sqrt{2}}\right)\right] dy\right) du \end{aligned} \quad (17)$$

This more complex function can be approximated by a stretched exponential function over a wide Q range:

$$F(x) \simeq \exp\left(-\left(\frac{x}{b}\right)^\beta\right) \quad (18)$$

with the parameters $b \simeq 1.354$ and $\beta \simeq 0.85$. For the evaluation of this experiment this approximation of $F(x)$ can be used.

3.3 Center of mass diffusion

With NSE spectroscopy the movements on length scales in the order of nanometer and time scales in the order of nanoseconds can be observed. This matches e.g. the center of mass

diffusion of macromolecules in solution or micelles. The mean square displacement of a particle is $\langle r^2(t) \rangle = 6D_{CM}t$ with the diffusion constant $D_{CM} = k_B T / (6\pi\eta R_G)$, where R_G is the hydrodynamic particle radius and η the viscosity (Stokes-Einstein-relation). The dynamic structure factor which is measured by NSE is then

$$I(Q, t)/I(Q, 0) = \exp(-1/6 \langle r^2(t) \rangle Q^2) = \exp(-D_{CM}Q^2t) \quad (19)$$

A simple diffusion therefore has a quadratic dependence on the the scattering vector Q .

4 Preparatory exercises

1. How fast do neutrons with a wavelength of 8 Å fly?
2. What is the value of the earth's magnetic field?
3. What is the magnetic field at the surface of a common permanent magnet?
4. How many mm fall neutrons on their way from the entrance of the spectrometer to the detector (about 7 m) due to gravity?
5. How many precessions does a neutron of $\lambda = 8$ Å perform in the main coils if the Fourier time is set to 20 ns? (Angle $\Psi = \gamma/v \int Bdl$).

5 Experiment procedure

5.1 The experiment itself

First, the function of the key components of the neutron spin-echo spectrometer will be explained and demonstrated.

The generation of the "Spin Echo" will be demonstrated with an auxiliary phase coil, wound around one of the main precession coils with a simple wire. With a laboratory DC-powersupply connected to this coil, the magnetic field inside this main coil is slightly varied. A fully symmetrical setup with identical magnetic path integrals in both main coils results in a maximum count rate at the detector. Increasing the current in the auxiliary coil from this point results in an additional phase shift of the neutron spin and thus the intensity varies from the maximum to a minimum and further to the next maximum and so on. In this way, the echo group is scanned.

The experimental sample under investigation is a polymer chain (PEP, polyethylenepropylene) with a molecular weight of 70 kg/mol in solution (deuterated decane). The PEP concentration is 3 wt %. The first experiment with the sample is to measure the elastic scattering by recording the spin-up and spin-down intensity at the detector.

- The coherent and incoherent scattering of the sample shall be extracted from this reading and plotted versus the scattering vector Q .

The dynamics of the sample is measured. For some selected scattering vectors Q , a series of Fourier times is measured for the sample, for a background sample containing everything but the objects under investigation, in this case the pure deuterated solvent (d-decane), and for an elastic scatterer as reference.

5.2 Data reduction

Each Fourier time is determined by measuring 2-3 oscillations of the echo bunch and fitting the theoretical curve (a cosine oscillation with a gaussian envelope) to the measured points. In short, the normalized amplitude of the fitted curve is the degree of polarization obtained in this measurement. This procedure is done with a program called `echodet`, which creates the files containing the intermediate scattering function $I(Q, t)/I(Q, 0)$.

5.3 Data evaluation

The $I(Q, t)$ vs. t is contained in the files `b_XXXXX` as ascii-data.

- Read in the data with some data treatment program (e.g. free software `qtikWS10`).
- Try to fit the data. First use a simple exponential function $I(Q, t) = A \exp(-\Gamma t)$ and determine the relaxation rate Γ . For diffusion like behaviour with the Stokes-Einstein diffusion coefficient, $\Gamma = DQ^2$ should be valid. Plot Γ/Q^2 vs. Q to check the validity of the model. It also allows for the determination of the hydrodynamic radius of the particle assuming a viscosity of d-decane of $\eta = 0.954 \times 10^{-3}$ kg/(ms).
- Use a stretched exponential function as model function: $I(Q, t) = A \exp(-[\Gamma t]^\beta)$ and determine the relaxation rate Γ and the stretching exponent β . The Zimm model would predict that the rate depends on the viscosity η as $\Gamma = k_B T / (6\pi\eta) Q^3$. What is the viscosity of d-decane? Does the Q -dependence of the model describes that of the data correctly (i.e. is $\Gamma/Q^3 = \text{const.}$)?

6 Experiment related exercises

Data evaluation (the bullet points in section 5):

1. Separate coherent and incoherent scattering from the elastic scan (diffnun) and plot it.
2. Evaluate the data containing $I(Q, t)/I(Q, 0)$ vs t with the models as described in the previous section and discuss the results.

General questions:

1. Why are no iron yoke magnets used in the construction of a NSE spectrometer?
2. What is the maximum field inside the main precession coils of the J-NSE?
3. What determines the resolution of the spin echo spectrometer?
4. How does the signal look like if the scattering is spin-incoherent? (Hint: in this case 2/3 of all neutron spins get flipped in the scattering process.)
5. What is the measured effect of the spin echo spectrometer?
6. What is measured finally?

References

- [1] F. Mezei, editor. *Neutron Spin Echo, Proceedings Grenoble 1979*, volume 128 of *Lecture Notes in Physics*. Springer, 1980.
- [2] D. Richter M. Monkenbusch, R. Schätzler. *Nucl. Instr. Meth. in Phys. Res. A*, 399:301–323, 1997.
- [3] D. Richter, M. Monkenbusch, A. Arbe, and J. Colmenero. *Adv. Polym. Sci.*, 174:1–221, 2005.

Contact

J-NSE

Phone: 089/289-14903

Web: <http://www.mlz-garching.de/j-nse/>

Olaf Holderer

Jülich Centre for Neutron Science, Outstation at MLZ
Forschungszentrum Jülich GmbH

Phone: 089/289-10707

e-Mail: o.holderer@fz-juelich.de

Web: <http://www.jcns.info>

Oxana Ivanova

Phone: 089/289-10730

e-Mail: o.ivanova@fz-juelich.de

Web: <http://www.jcns.info>

KWS-1 & KWS-2

Small Angle Neutron Scattering

H. Frielinghaus, M.-S. Appavou



Contents

1	Introduction	3
2	Preparing solutions in Water	3
3	The Measurement at KWS-1 and/or KWS-2	4
4	Evaluation of the Scattering Data: Absolute Calibration	4
5	Evaluation of Lysozyme Scattering Curves	4
6	Evaluation of the Polymer Scattering	5
7	Preparatory Exercises	6
	Contact	7



Fig. 1: Representation of the protein lysozyme, which has a very compact form.

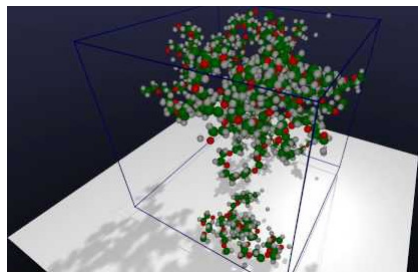


Fig. 2: Molecular dynamics conformation of poly ethylene oxide in solution.

1 Introduction

The objective of this lab course is to clarify the essential concepts of small-angle neutron scattering. Structures are only visible by a scattering experiment if there is an appropriate contrast. For neutrons one often uses the exchange of ^1H by ^2H , i.e. deuterium. The contrast of this lab course is achieved by using heavy water (D_2O) as solvent. The materials (solutes) are natural ones having normal protons.

The globular, compact lysozyme (Fig. 1) appears in chicken eggs and has anti-bacterial function. The molecule is charged, which leads to repulsive interactions. So there is a short range order, and the distance between the molecules can be determined.

The other molecule is the synthetic poly ethylene oxide (Fig. 2) with the chemical formula of $[-\text{CH}_3-\text{CH}_2-\text{O}-]_n$. It is one of the simplest water soluble polymers. The hydrogen bonds of the oxygen are responsible for attractive interactions between water and the polymer. The molecules form rather dilute coils in solution and the overall dimension of the coil will be determined by SANS. Furthermore, the fractal structure of the coil will be determined.

2 Preparing solutions in Water

A lysozyme solution of 0.02g per ml of water must be prepared. We will weigh 0.02g of Lysozyme and put it into a new Packard glas. With an Eppendorf pipette we will add exactly 1 ml D_2O . These pipettes are extremely accurate with respect to the volume. From the solution about 0.5 to 0.6ml are transferred to Hellma quartz cuvettes, which are 1mm thick. For the later evaluation we need a highly accurate concentration. So all weights need to be written down as exactly as possible.

For the poly ethylene oxide solution we chose the same concentration. Since the polymer exists

in small platelets the tiny amount of polymer will not be that accurately prepared. Corrections can be either done by choosing a different volume of heavy water or by just writing down the exact weights. However, stay below 0.04g/ml for the concentration!

3 The Measurement at KWS-1 and/or KWS-2

These two solutions are now being measured in the small-angle neutron scattering instrument KWS-1 (or KWS-2). The wavelength of neutrons is set to 7\AA . The collimation is fixed to 8m. The samples are placed as close as possible to the detector, to measure the largest Q values possible. Both samples will be measured at detector distances 2m and 8m. The offset between the sample position and the detector of about 30cm leads to effective detector distances of about 1.7m and 7.7m.

The sample holder will be filled with the two samples. In addition, the empty beam and a plexiglass plate are measured for absolute calibration. For a good statistical measurement the following times are set: 8m detector distance for 20min, and 2m detector distance 10min. The total measuring time for the 4 positions will be about 2 hours. The measurement is typically started before lunch, and can be evaluated in the afternoon. It is quite likely that an internal employee will start separate measurements during the afternoon until the next morning in order to use the valuable measuring time overnight.

4 Evaluation of the Scattering Data: Absolute Calibration

The measured data is raw data at first and describes the intensity on the detector. The data has to be corrected for the effectiveness of the different detector channels. Then the empty beam measurement is subtracted to account for the zero effect of the instrument. Then the intensities are expressed as absolute units using Eq. 5.5 and are radially averaged, because for the isotropic scattering samples, the intensity does not depend on the polar angle. To perform all these steps we will be using a software available in our institute, called QtiKWS. However, since the understanding of the Eq. 5.5, as such, is more important than the exact technical understanding of the evaluation, the results are produced relatively quickly by the software, namely, $d\Sigma/d\Omega$ as a function of the scattering vector Q for our samples. This data will be provided for the students to do the final evaluation. In the following, this evaluation is described.

5 Evaluation of Lysozyme Scattering Curves

The position of the maximum Q_{\max} provides information on the typical distance of the proteins in solution. This can be calculated to $\ell = 2\pi/Q_{\max}$. Knowing the weight of the protein in water (0.02g/cm^3) there is an alternative way to calculate the average distance. The molar mass of the protein is $1.43 \times 10^4\text{g/mol}$. The number density of the protein is therefore $n/V = 0.02\text{g/cm}^3 / (1.43 \times 10^4\text{g/mol}) = 1.40 \times 10^{-6}\text{mol/cm}^3 = 8.42 \times 10^{-7}\text{\AA}^{-3}$. For a simple cubic packing the typical distance is given by $\ell = \sqrt[3]{V/n}$. For a hexagonal close packed lattice the

typical distance is $\ell = \sqrt[6]{16/27} \sqrt[3]{V/n}$. This distance is the minimum distance of the planes important for the scattering experiment, and the next neighbor distance of the hexagonal c.p. lattice is $\sqrt{3/2} \ell = \sqrt[6]{2} \sqrt[3]{V/n}$. Both calculated distances of the cubic and hexagonal structure are to be compared with the measured one.

6 Evaluation of the Polymer Scattering

In a first step we have to prepare the scattering data for background subtraction. We plot the original data of the two detector distances in a log-log plot, i.e. $\log_{10}(d\Sigma/d\Omega) \rightarrow \log_{10} Q$. After this, we will see a plateau at high Q which indicates the constant incoherent scattering. Taking the average of the last (say 10) points will give us the estimate of the background. A new column with the background subtracted will be generated for the 8m and 2m measurements. Finally, the two data sets should be combined to yield a single data set.

Now, we will aim at the overall appearance of the chain, i.e. we will determine the chain dimension. For this purpose the Guinier approximation can be applied. The general appearance of the Guinier scattering law was already given in eq. 5.35 and reads:

$$\frac{d\Sigma}{d\Omega}(\mathbf{Q} \rightarrow 0) = \frac{d\Sigma}{d\Omega}(0) \cdot \exp\left(-\frac{1}{3}Q^2 R_g^2\right) \quad (1)$$

For this purpose we plot the logarithm of the background corrected intensity against the square of the scattering vector, i.e. $\ln(d\Sigma/d\Omega) \rightarrow Q^2$. The highest Q will lead to large values that we are not interested in. So the plot has to be truncated to the rather small Q , say $Q^2 = 0.4 \times 10^{-4} \text{Å}^{-2}$. Here, we do a linear regression and take the slope S as a result only. It has the units Å^2 . From this we can calculate the radius of gyration using $R_g = \sqrt{-3S}$. From previous measurements we know that it is roughly 60Å large.

For the fractal structure we plot the data in a log-log plot again (background corrected). There is the Guinier region indicated by flat scattering at low Q . At high Q the data will have very large noise, and maybe negative values might appear from the subtraction. In the middle, the scattering should be linear, indicating a power law characteristic for fractal structures. Again, we use a linear regression to determine the slope α . From the ideal polymer without interactions we learned that the exponent would read $\alpha = 2$ (see eq. 5.50). When taking the attractive interactions of the solvent into account, the exponent would be rather $\alpha = 1.70$. The reciprocal value α^{-1} is called Flory exponent and takes the ideal values of 0.5 or 0.588 for non-interacting chains and chains in a good solvent, respectively. Please make your own judgement!

7 Preparatory Exercises

(I) Lysozyme in D₂O

The first sample of the Neutron Lab Course at the SANS instrument KWS-1 (KWS-2) will be Lysozyme in heavy water (D₂O). This protein is rather globular (diameter ca. 5 nm). The Coulomb interactions of this charged molecule lead to liquid-like short-range-ordering. This will be observed in the SANS scattering experiment by a correlation peak. Simple estimations will be made now:

1. Give the connection between the number density ϕ and the unit cell parameter assuming a simple cubic lattice!
2. The chemical concentration c is usually given in g/L or mg/ml. The molar mass of the molecule is 14307 g/mol. What is the connection between the chemical concentration and the number density?
3. The correlation peak appears at a scattering vector Q_{\max} . How would it relate to the unit cell parameter of a simple cubic lattice? What is the dependence of Q_{\max} as a function of the chemical concentration c ?
4. Please rationalize the relations of the hexagonal close packed lattice with respect to the cubic packing! The spacing of the planes is shorter by a value of roughly 0.916 (larger Q value compared to cubic). The nearest neighbor has a larger distance of ca. 1.122 times the cubic packing.

(II) Polymer in Solution

We will look on the overall dimension of the chain and on the fractal structure of the chain.

1. The Appendix B derived the Guinier scattering law for any shape of particles while in the main manuscript the first application was the compact sphere. How has the compactness of a polymer in a good solvent to be seen? Is there any restriction for the Guinier scattering for polymers?
2. At large Q we observe a constant background from incoherent scattering. The hydrogen atom has a incoherent cross section of $80 \times 10^{-24} \text{cm}^2$, and the deuterium atom $2 \times 10^{-24} \text{cm}^2$. The concentration of hydrogen from the polymer is roughly 50 times smaller than the concentration of deuterium from the heavy water. On the basis of these numbers estimate the ratio of background from the polymer and the solvent!
3. The fractal structure means that looking inside a coil still finds the situation of the connectivity of a chain on smaller length scales compared to the overall chain. The chain is self-similar on length scales (between the overall coil dimension and the monomer dimension). The different exponents α of 2 and 1.7 for ideal chains and polymers in a good solvent describe different compactness of the structure. Rationalize the difference between a non-interacting chain and a chain that “feels” its own presence!

Contact

KWS-1 & KWS-2

Phone: +49-89-289-14324 & +49-89-289-14326

Web: <http://www.mlz-garching.de/kws1>
<http://www.mlz-garching.de/kws2>

Henrich Frielinghaus

Jülich Centre for Neutron Science
Forschungszentrum Jülich GmbH
at Heinz Maier-Leibnitz Zentrum
Lichtenbergstrasse 1
D-85747 Garching, Germany

Phone: +49-89-829-10706

e-Mail: H.Frielinghaus@fz-juelich.de

Aurel Radulescu

Phone: +49-89-829-10712

e-Mail: A.Radulescu@fz-juelich.de

Ida Berts

Phone: +49-89-289-10758

e-Mail: I.Berts@fz-juelich.de

Artem Feoktystov

Phone: +49-89-289-10746

e-Mail: A.Feoktystov@fz-juelich.de

Gaetano Mangiapia

Phone: +49-89-289-11673

e-Mail: G.Mangiapia@fz-juelich.de

Marie-Sousai Appavou

Phone: +49-89-289-10747

e-Mail: M.S.Appavou@fz-juelich.de

Noemi Szekely

Phone: +49-89-289-10739

e-Mail: N.Szekely@fz-juelich.de

KWS-3

Very Small Angle Neutron Scattering Diffractometer with Focusing Mirror

Vitaliy Pipich

Jülich Centre for Neutron Science
Forschungszentrum Jülich



Contents

1	Introduction.....	3
2	VSANS applications.....	4
3	Preparatory Exercises	4
4	Experiment Procedure	5
5	The experiment and data reduction.....	7
6	Experiment-Related Exercises.....	7
	References	9
	Contact	10

1 Introduction

Ultra small angle (USANS) and small angle neutron scattering (SANS) experiments are performed by two different types of instruments to cover a combined Q-range from 10^{-5} \AA^{-1} up to 1 \AA^{-1} . Double crystal diffractometers are used for USANS experiments, whereas the "standard" SANS experiment is performed using a pinhole camera. In principle, the Q-range of both instrument classes overlaps. Typical USANS instruments like S18 (ILL) or PCD (NIST) may reach maximum Q-vectors of $5 \cdot 10^{-3} \text{ \AA}^{-1}$. The disadvantage of these instruments is that they do not allow taking a full area image on a 2D position sensitive detector. On the other hand, the well-known pinhole instrument D11 at Institut Laue-Langevin (France) reaches a minimum Q-vector of $3 \cdot 10^{-4} \text{ \AA}^{-1}$ by use of largest possible wavelength 22 \AA and sample-to-detector distances ($>40 \text{ m}$). But the required instrumental settings push both types of instruments to their limits, mainly due to signal-to-noise level and the reduced flux at sample position. The use of neutron lenses as additional elements of a pinhole SANS instrument has been tested to overcome this intensity problem [1].

An alternative design is realized by the KWS-3 instrument [2]. The principle of this instrument is a one-to-one image of an entrance aperture onto a 2D position-sensitive detector by neutron reflection from a double-focusing elliptical mirror. It permits to perform SANS studies with a scattering wave vector resolution between 10^{-4} and 10^{-3} \AA^{-1} with considerable intensity advantages over conventional pinhole-SANS instruments and double crystal diffractometers. Therefore it perfectly bridges the "Q-gap" between USANS and SANS: Very Small Angle Scattering (VSANS). The increasing need for these intermediate Q-vectors arises from the growing interest in biological and colloidal samples, which partially deal with length scales in the μm range. An investigation of the multilevel structures in partially crystalline polymer solutions performed using a combination of those three above depicted types of SANS instruments can be found in [3].

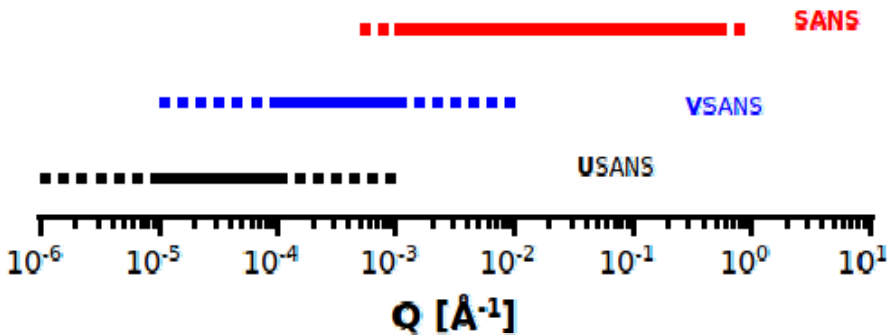


Figure 1: Focused VSANS fills space between USANS (double crystal diffractometer) and classical SANS instruments.

The main innovation and challenge of KWS-3 was to build a large mirror having a shape as close as possible to an ellipsoid and with a surface roughness less than 5 \AA . The mirror is a

1.2 m long, 0.12 m wide and 0.05m thick toroidal double focusing mirror of 11 m focal length. At such a short mirror length with respect to the focal length, the toroidal shape is a good enough approximation to an elliptical shape. The reflection plane has been chosen to be horizontal, reducing the deterioration of the image due to gravity. A photo of the mirror is given in Figure 1.

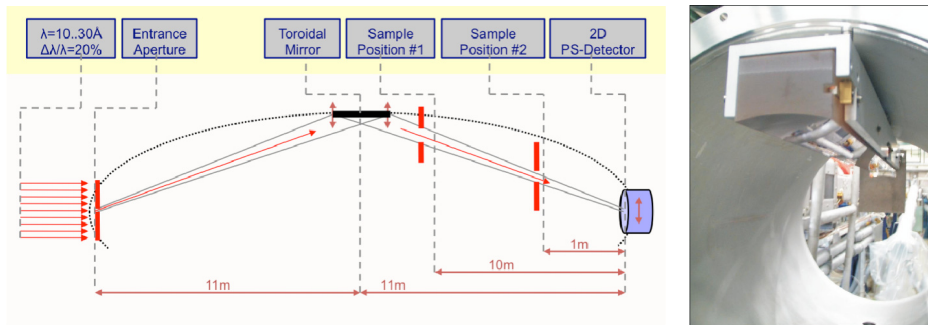


Figure 2:(left) layout of KWS-3;(right) toroidal mirror installed in vacuum its chamber.

KWS-3 is optimized for very small angle scattering range from 10^{-4} to $3 \cdot 10^{-3} \text{ \AA}^{-1}$. For last cold source filling and instrument configuration the flux at the sample position (and detector) is near **11500** counts per full sample area by use 12.5 \AA wavelength with 20% wavelength spread, $2 \times 2 \text{ mm}^2$ entrance aperture and $20 \times 100 \text{ mm}^2$ beam size sample-to-detector distance at 9.5 meters.

2 VSANS applications

All applications of the classical SANS could be investigated by VSANS by taking into account Q-resolution of VSANS. The conventional fields of application of very small angle scattering studies are:

- particles in solution [protein aggregates, polymers, micelles, ceramics];
- porous materials [cement, paste, rocks, coal etc.];
- inhomogeneous metallic alloys;
- bulk samples with artificial regular structure [phase gratings];

and other inhomogeneities on a size range from 50 nm to 5 μm , often in addition to SANS spectra, but also diffraction, reflection and refraction studies on surfaces.

3 Preparatory Exercises

1. The contrast variation (CV) is a very important feature of the neutron scattering. What is the scattering length density (SLD) ρ ? How to calculate the SLD? What is the definition of the scattering contrast $\Delta\rho$? How to carry out the contrast variation experiment in case of an aqueous solution of particles?

2. The standard Q-range of KWS-3 is from 10^{-4} to $3 \cdot 10^{-3} \text{ \AA}^{-1}$. What the size of particles could be investigated in this Q-range? What are the form factor $P(Q)$ and structure factor $S(Q)$? In which case the scattering intensity $d\Sigma/d\Omega(Q)$ could be represented as a product of the structure factor and form factor $d\Sigma/d\Omega(Q) = d\Sigma/d\Omega(0) \cdot P(Q) \cdot S(Q)$? What is the physical “content” of the forward scattering $d\Sigma/d\Omega(0)$ [$I(0)$]?
3. The standard wavelength at KWS-3 is 12.5 \AA . What are disadvantages of this wavelength? What should we correctly select before sample preparation?
4. What is the difference between pine-hole SANS and focused SANS? Why the beam size at KWS-3 is 20 cm^2 ?

4 Experiment Procedure

Within the frame of this practicum we will explore aqueous solution of monodisperse polystyrene (PS) microspheres with diameter 8000 \AA and the initial concentration 1% of particles in H_2O . In future, this sample will be used at KWS-3 as “a standard sample” to check the performance of instrument, absolute calibration, instrument resolution.

In Table 1 there is collected information about PS microspheres obtained from the producer; additionally all necessary information about H_2O and D_2O is listed there.

Table 1. Parameters of used components

	Polystyrene Spheres	H_2O	D_2O
Scattering Length Density [\AA^{-2}]	$1.41 \cdot 10^{-6}$	$-0.56 \cdot 10^{-6}$	$6.50 \cdot 10^{-6}$
Density, 20°C [g/cm^3]	1.05	1.0	1.05
Radius [\AA]	4000 ± 45		

The contrast variation is proposed to proceed simply by step-by-step adding of D_2O to the initial H_2O solution of spheres. To estimate how much of D_2O we should add, the simulation of the forward scattering should be done as function of D_2O concentration:

$$\frac{d\Sigma}{d\Omega}(0) = \Phi_{\text{Spheres}} V_{\text{Spheres}} (\rho_{\text{Spheres}} - \rho_{\text{Water}})^2,$$

where V_{Spheres} is volume of PS spheres, ρ_{Spheres} SLD of PS spheres, ρ_{Water} SLD of $\text{D}_2\text{O}/\text{H}_2\text{O}$ mixture, Φ_{Spheres} volume fraction of PS spheres in $\text{D}_2\text{O}/\text{H}_2\text{O}$ mixture. We could rewrite the above-mentioned equation in terms of Φ_0 and $\Phi_{\text{D}_2\text{O}}$, the volume fraction of PS spheres in the initial H_2O solution and volume fraction of D_2O in $\text{D}_2\text{O}/\text{H}_2\text{O}$ mixture respectively:

$$\frac{d\Sigma}{d\Omega}(0) = \frac{\Phi_0(1 - \Phi_{\text{D}_2\text{O}})}{1 - \Phi_0 \Phi_{\text{D}_2\text{O}}} V_{\text{Spheres}} [\rho_{\text{Spheres}} - \rho_{\text{H}_2\text{O}} - \Phi_{\text{D}_2\text{O}}(\rho_{\text{D}_2\text{O}} - \rho_{\text{H}_2\text{O}})]^2.$$

In Figure 3 the forward scattering $d\Sigma/d\Omega(0)$ as a function of $\Phi_{\text{D}_2\text{O}}$ and Φ is plotted. At the starting point of the experiment ($\Phi_{\text{D}_2\text{O}}=0$) we have PS spheres in pure H_2O and maximal volume fraction of spheres $\Phi_{\text{Spheres}} = \Phi_0 = 1\%$. Minimum of the plotted curve corresponds to the matching point of PS spheres in water. In Table 2 seven points around matching concentration are labeled with “CV” mark. In case of CV, from the scattering curves of above-mentioned samples we need to extract only “integral” parameter forward scattering to

extract information about minimum of the forward scattering, and plot it as function of D₂O content.

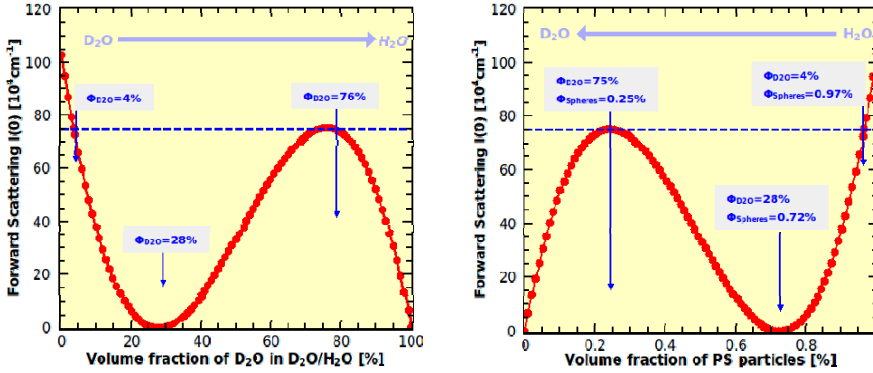


Figure 3. Forward scattering as a function of Φ_{D2O} and Φ .

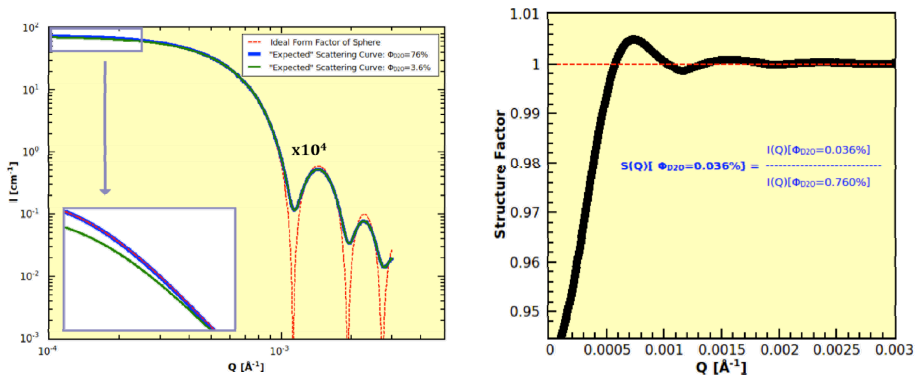


Figure 4: Expected results. (Left) the scattering signal in case of $\Phi_{D2O}=0.04$ and 0.76 . In the amplified inset is the small angle part of the calculated scattering curves. In case of $\Phi_{D2O}=0.04$ there is clear suppression of the forward scattering due to the hard sphere interactions. Calculated scattering curve in case of the sample with $\Phi_{D2O}=0.76$ shows no interaction term. Red curve is pure form factor of PS spheres without taking into account instrumental resolution function. (Right) Ration between $\Phi_{D2O}=0.04$ and $\Phi_{D2O}=0.76$ is plotted here. So the forward scattering and form factor of both sample are the same, and in case of $\Phi_{D2O}=0.76$ sample $S(Q)=1$, therefore this ratio is the structure factor of $\Phi_{D2O}=0.04$ sample.

Next step is the investigation PS spheres in case of sample with D₂O content 76% [PS content 0.25%]. This point is located at the local maximum (see Figure 3). At this level of the dilution the structure factor is definitely undetectable. Please read carefully caption of Figure 4 to understand the logic of planned experiment.

Table 2. Samples for practicum; CV: samples for the contrast variation; FF, SF: sample for form and structure factor determination.

Φ_{D2O}	0 ^{CV}	3.6 ^{FF, SF}	10 ^{CV}	20 ^{CV}	30 ^{CV}	40 ^{CV}	50 ^{CV}	60 ^{CV}	76 ^{FF}
$\Phi_{Spheres}$	1.00	0.96	0.9	0.8	0.7	0.6	0.5	0.4	0.24
$I(0)[10^4 \text{cm}^{-1}]$	103	75.2	38	6.5	0.47	12.01	33.2	55.9	75.2

5 The experiment and data reduction

All samples listed in Table 2 we will measure with (Sample) and without (Sample-DB) beamstop. The first one should be measured much longer than the second one. Additionally the empty cell [with (EC) and without (EC-DB) beamstop] and the black current (BC) run will be measured and used for data reduction of all datasets.

What to measure?

$I_{\text{Sample}}, I_{\text{Sample-DB}}, I_{\text{EC}}, I_{\text{EC-DB}}, I_{\text{BC}}$ [counts per current pixel, normalized by monitor]

Sample transmission:

$$T = I_{\text{Sample-DB}} / I_{\text{EC-DB}}$$

Empty cell and black current subtraction:

$$I = (I_{\text{Sample}} - I_{\text{BC}}) - T \cdot (I_{\text{EC}} - I_{\text{BC}})$$

Absolute calibration:

$$\frac{d\Sigma}{d\Omega}(Q) = \frac{I(Q)}{d \cdot T \cdot \varepsilon_D \cdot \langle I_{\text{EC-DB}} \rangle \Delta\Omega(Q)}$$

where d sample thickness, T sample transmission, ε_D detector efficiency, $\Delta\Omega$ solid angle per current pixel, $\langle I_{\text{EC-DB}} \rangle$ counts on sample.

6 Experiment-Related Exercises

Within our “one-day-experiment” at KWS-3 it would be nice to get as much as possible information about above mentioned sample, like:

- the form factor $P(Q)$ of PS spheres from sample with $\Phi_{D2O}=0.76$; “real” radius R and polydispersity of the PS microspheres;
- the structure factor $S(Q)$ in case of $\Phi_{D2O}=0.04$ and decide about the interactions between spheres: could we neglect the structure factor $S(Q)$ during data analysis?

- c) the scattering length density of PS spheres by $\text{H}_2\text{O}/\text{D}_2\text{O}$ contrast variation. At matching point, the SLD of microspheres and water are equal. Polystyrene in microspheres is amorphous or crystalline?

References

- [1] Eskilden, M. R. et al., *Nature* 391, 563 (2000);
Frielinghaus, H. et al., *J. Appl. Cryst.* 42, 681 (2009);
- [2] Alefeld, B. et al., *Physica B* 283, 330 (2000);
Kentzinger, E. et al., *Physica B* 350, e779 (2004);
Goerigk, G. et al., *J. Appl. Cryst.* 44, 337 (2011);
- [3] Radulescu A. et al., *Macromolecules* 39, 6142 (2006)

Contact

KWS-3

Phone: 089/289-14325
Web: <http://www.mlz-garching.de/kws-3>

Vitaliy Pipich

Jülich Centre for Neutron Science JCNS
Forschungszentrum Jülich GmbH
Outstation at FRM II
Phone: 089/289-10710
e-Mail: v.pipich@fz-juelich.de
Web: <http://iffwww.iff.kfa-juelich.de/~pipich>


Zhendong Fu

Jülich Centre for Neutron Science JCNS
Forschungszentrum Jülich GmbH
Outstation at FRM II
Phone: 089/289-10716
e-Mail: z.fu@fz-juelich.de

TREFF

Reflectometer

S. Mattauch and U. Rücker
Jülich Centre for Neutron Science
Forschungszentrum Jülich

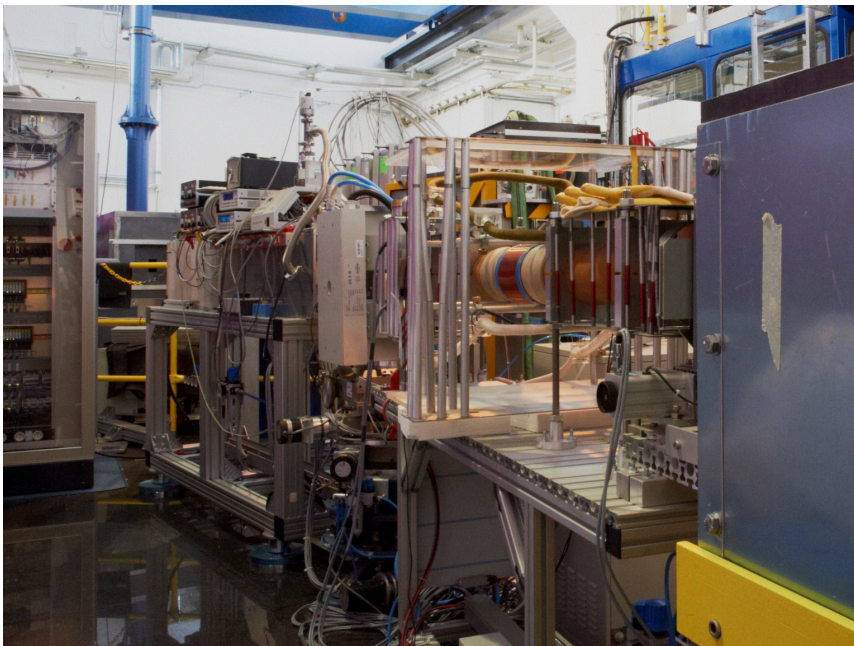

Contents

1	Introduction	3
2	Preparatory Exercises	3
3	Experiment Procedure	4
3.1	The experiment itself	4
3.2	Data reduction	5
3.3	Data evaluation	5
4	Experiment-Related Exercises	6
	References	7
	Contact	8

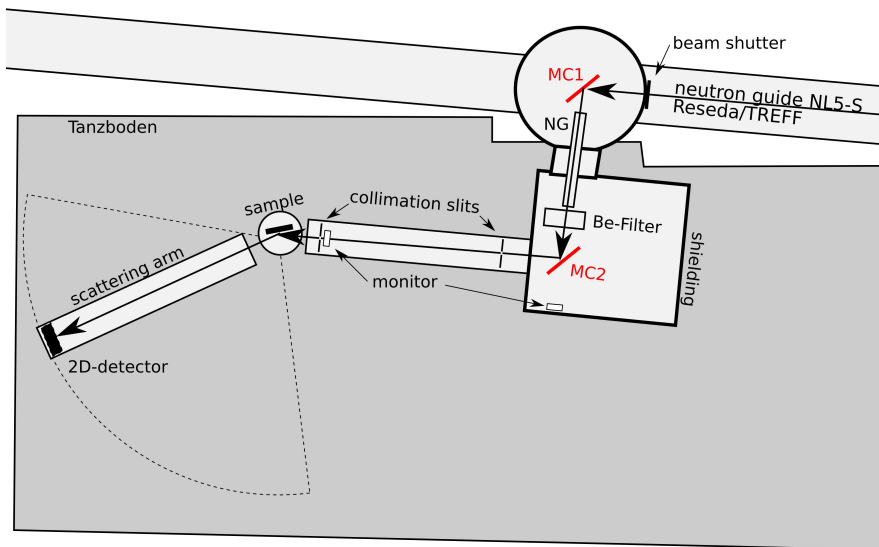


Fig. 1: Sketch of the reflectometer TREFF@NOSPEC in top view.

1 Introduction

The neutron reflectometry TREFF@NOSPEC at the neutron guide NL5-S is part of the neutron guide laboratory at the research reactor FRM II in Garching. TREFF is a joint facility of JCNS and the neutron optics group of FRM II. It is used for the investigation of magnetic layered structures as well as neutron optical components for the installation and improvement of neutron scattering instruments.

Figure 1 depicts the neutron reflectometer TREFF in the neutron guide hall of the FRM II research reactor. Essentially, it consists out of a double monochromator, the collimation path, the sample table with several stages of translation and rotation and, finally, the scattering arm with a position sensitive detector. The distance between the collimation slits is 1820mm and 450mm between the second slit and the centre of rotation of the sample table. For this experiment the wavelength is set to $\lambda=4.73 \text{ \AA}$.

2 Preparatory Exercises

The following questions will be asked during the practical course at TREFF:

1. In the sketch (Figure 1 of the instrument you will find a Be-filter and a NG (neutron guide) between the MC1 and MC2. What are they used for?

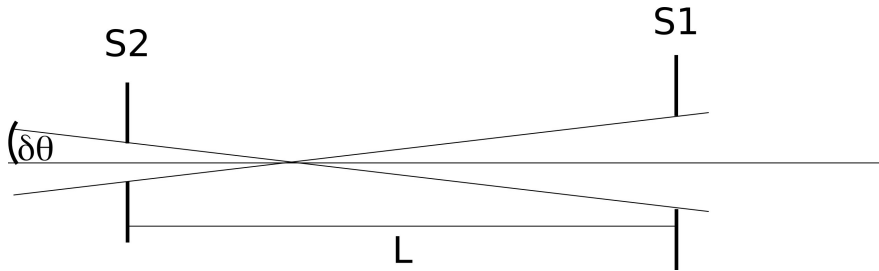


Fig. 2: This drawing should help you to solve question 5.

2. In the introduction the used wavelength was given with $\lambda=4.73 \text{ \AA}$. Which other wavelength are possible and how do you achieve these?
3. Depict a reflectivity curve of a substrate only
4. Depict a reflectivity curve of a substrate plus a layer
5. Calculate the divergence of a beam passing two slits S1 and S2 in a distance of L (see Figure 2)
6. Calculate the angle of collimation of the neutron beam to sufficiently resolve reflectivity oscillations of a 80nm thick monolayer on a substrate. What slit sizes follow for this reflectometer

3 Experiment Procedure

The aim of this experiment is the investigation of a nickel monolayer deposited on a glass substrate with unknown composition. Using neutron reflectometry the thickness of the nickel layer should be determined.

1. Perform a reflectivity experiment on the sample's back side and analyse the critical angle. To get sufficient collimation of the neutron beam, 0.6mm slit size for S1 and S2 should be taken.
2. Take the reflectivity curve of the Ni-monolayer system with the suitable collimation angles, so speaking the slit size for S1 and S2 calculated in the section before
3. Do like 3) but with a slit size of 3mm for S1 and S2.

3.1 The experiment itself

We (in the end it will be you) will mount the sample on the sample table and pre-align it with an appropriate tool (what could it be) parallel to the neutron beam. After some alignment scans

with the neutron beam we will measure the reflectivity curve step by step of the sample (see chapter Experiment Procedure).

3.2 Data reduction

The instrument saves the number of counts as a function of scattering angle.

3.3 Data evaluation

For systems such as multilayers the scattered intensity is determined by the difference in the potential of each layer (contrast). The potential is given by the **scattering length density** $\rho_{sld} = \sum_j b_j \rho_j$ with the scattering lengths b_j and the particle number densities ρ_j . The index j runs over all kind of atoms of the layer. The scattering length density is comparable to the optical density in light optics.

The **refraction index** of each layer is given by

$$n \gg 1 - \frac{\lambda^2}{2\pi} \rho_{sld} = 1 - \delta$$

With the **angle of total external reflection** $\Theta_c \sim \sqrt{2\delta}$, which is usually small, it follows

$$k_{c,z} = k \sin(q_c) \gg k q_c = \frac{2\pi}{\lambda} \sqrt{2 \frac{\lambda^2}{2\pi} \rho_{sld}} = \sqrt{4\pi \rho_{sld}}$$

for the **critical wave vector**. For a monolayer system the **reflected amplitude** of each interface $r_{f,1}$ and $r_{f,2}$ can be calculated by the Fresnel formulae (Equation 16 in chapter 12 of the lectures book).

Neglecting roughness at the sample surface and at the interface between layer and substrate, for the amplitude at the surface one gets

$$r_{f,1} = \frac{k_{z,vac} - k_{z,lay}}{k_{z,vac} + k_{z,lay}} \quad \text{and at the interface} \quad r_{f,2} = \frac{k_{z,lay} - k_{z,sub}}{k_{z,lay} + k_{z,sub}}$$

with

$$k_{z,vac} = k \sin(q) \quad , \quad k_{z,lay} = \sqrt{k_{z,vac}^2 - 4\pi \rho_{sld,lay}} \quad \text{and} \quad k_{z,sub} = \sqrt{k_{z,vac}^2 - 4\pi \rho_{sld,sub}}$$

The superposition of both amplitudes yields the reflected amplitude of a monolayer sample

$$R = [r_{f,1} + r_{f,2} \exp(2ik_{z,lay}d)] \frac{\exp(-2ik_{z,vac}d)}{[1 + r_{f,1}r_{f,2} \exp(2ik_{z,lay}d)]}$$

with the film thickness d . The **reflected intensity** is given by the mean square of R . For $k_{z,vac} > 3k_{c,z}$ the intensity can be calculated in **Born approximation** by

$$|R|^2 \gg \frac{\pi^2}{k_{z,vac}^4} [\rho_{sld,lay}^2 + (\rho_{sld,lay} - \rho_{sld,sub})^2 + 2\rho_{sld,lay}(\rho_{sld,lay} - \rho_{sld,sub}) \cos(2k_{z,vac}d)]$$

4 Experiment-Related Exercises

1. calculate from the reflectivity curve of the glass substrate the scattering length density $\rho_{sld,sub}$
2. Describe the differences and explain them between the measurement of the Ni monolayer with the 3mm slit and the slit size you have calculated.
3. Calculate the scattering length density $\rho_{sld,sub}$ of the Ni monolayer using:
molar volume $V_{Ni}=6.59 \text{ cm}^3 \text{ mol}^{-1}$
Avogadro number $N_L=6.02 \cdot 10^{23} \text{ mol}^{-1}$
coherent scattering length $b_{Ni}=10.3 \text{ fm}$
4. Determination of the thickness d of the Ni monolayer using the reflectivity formula in Born approximation. At first, estimate d based on the distance of the fringes of the reflectivity (see Data evaluation chapter).

References

Your lecture book of the year

Contact

TREFF

Phone: 089/289-10768

Stefan Mattauch

Jülich Centre for Neutron Science JCNS

Forschungszentrum Jülich GmbH

Phone: 089/289-10709

e-Mail: s.mattauch@fz-juelich.de

Alexandros Koutsoumpas

Jülich Centre for Neutron Science JCNS

Forschungszentrum Jülich GmbH

Phone: 089/289-11674

e-Mail: a.koutsoumpas@fz-juelich.de

Sabine Pütter

Jülich Centre for Neutron Science JCNS

Forschungszentrum Jülich GmbH


Phone: 089/289-10742

e-Mail: s.puetter@fz-juelich.de

TOFTOF

Time-of-flight spectrometer

L. Silvi, S. Busch, T. Unruh and W. Lohstroh

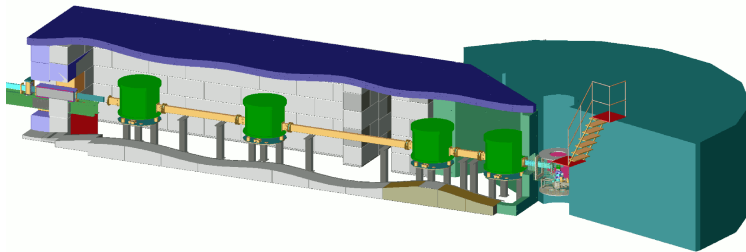

Contents

1	Introduction	3
2	Basics	4
2.1	The neutron source FRM II	4
2.2	The time-of-flight spectrometer TOFTOF	4
3	Theory	6
3.1	Cross sections	6
3.2	Principle of a scattering experiment	7
3.3	Correlation & scattering functions	8
4	Experiment	11
4.1	The system	11
4.2	Modelling the motions	11
4.3	The experiment itself	12
4.4	Data reduction	12
4.5	Data evaluation	14
5	Questions to be answered <i>before</i> the experiment	14
6	Questions to be answered <i>during</i> the experiment	14
7	Constants	16
	References	17
	Contact	18

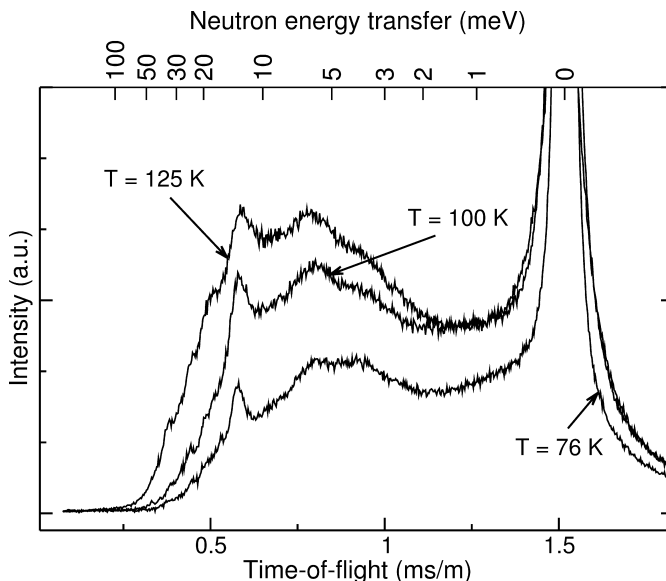


Fig. 1: Neutron time-of-flight spectrum of pentafluorotoluene, taken from [3]. Elastic scattering happens at energy transfer zero, quasielastic scattering in a region of approximately 0 ± 1 meV, inelastic scattering at larger energy transfers.

1 Introduction

Scattering experiments are carried out in order to obtain information about the structure and dynamics of the studied systems (e. g. crystals, liquids, nanoparticles). Optical microscopes are simpler to understand and operate but their resolution is limited by the wavelength of light. There are only few techniques which give access to the length scale of molecules and atoms. Of those, one of the most important is scattering.

There are several kinds of scattering experiments, depending on the subject matter. In this experiment we want to introduce you to *quasielastic neutron scattering* (QENS). Quasielastic scattering is referring to a broadening of the elastic line in a spectrum. The extend of this broadening is approximately 1 meV. Whereas in inelastic scattering (which will not be further discussed in this experiment), discrete maxima or bands appear clearly separated from the elastic line. While one can gain information about the structure or periodic motions (i. e. phonons) of the sample using *diffraction* or *inelastic scattering*, respectively, it is possible to analyse non-periodic motions (e. g. diffusion) with quasielastic scattering.

Prior to the experiment, you should read and understand these instructions, since you won't have much time to do so during the experiment. Along with this you should also work out the question section. In the following, we will first follow the path of the neutrons from the source over the sample to the detector. Afterwards, the theory of scattering will be roughly introduced, so that one can understand which information can be obtained from the scattered neutrons. Thereon the specific experiment will be explained.

To carry out the experiment, you should bring this introduction, your answers to the questions, paper and a pen. After having started the measurement of the reference sample, we will show you the spectrometer TOFTOF. Afterwards we will prepare a sample, which we then will measure. Finally, we will evaluate the data together.

2 Basics

2.1 The neutron source FRM II

In general there are two techniques in order to “produce” neutrons – spallation and nuclear fission. During spallation, huge nuclei (e. g. lead) are bombarded with protons, subsequently split and, among others, emit neutrons. The FRM II is a nuclear reactor used as a neutron source. Here, ^{235}U captures a thermal neutron and thereby becomes unstable. The nucleus fissures and, among others, emits three fast neutrons.

These fast neutrons must be slowed down (moderated) to thermal energies, that is room temperature, in order to initiate a new fission. One neutron is needed for the fission, while the others will be used for the neutron scattering experiments. The moderation occurs in D_2O of about 300 K which encloses the core.

In order to further slow down the neutrons, and thereby match their energies to the ones of atomic motions, a tank containing liquid D_2 at 25 K is located close to the fuel element. From this *cold source* several neutron guides lead the neutrons to the instruments. Inside these guides, the neutrons are transported by total reflection at the inner walls. The time of flight spectrometer TOFTOF is located at the end of neutron guide 2a in the neutron guide hall.

2.2 The time-of-flight spectrometer TOFTOF

The *cold neutrons* move with a velocity of several hundred m/s. Hence one can determine the kinetic energy of the neutrons comfortably by a time of flight (TOF) measurement along a certain distance. If one sets the initial energy of the neutrons before the scattering event to a well-known value and measures the final energy (or velocity) after the scattering process, the energy transfer can be determined. Since the position of the detectors is fixed, the scattering angle is also known.

During time of flight spectroscopy the energy transfer is measured by a time of flight measurement of the neutrons. The advantage of the time of flight technique is that a huge range of momentum and energy transfer can be captured simultaneously.

TOFTOF is a multi chopper time of flight spectrometer with direct geometry [4]. This means that all neutrons have (more or less) the same energy before interacting with the sample. After being scattered by the sample, the energy transfer can be determined. Both, the tuning of the energy of the incident neutrons (their wavelength) and the determination of the energy of the scattered neutrons is done by time of flight.

The neutrons are directed to the spectrometer through a neutron guide, which has a supermirror coating. The end of the guide is double focusing.

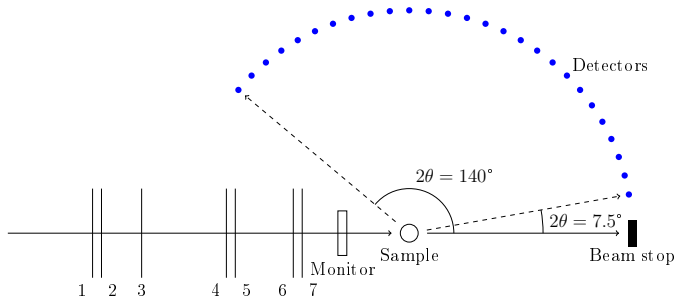


Fig. 2: Schematic drawing of TOFTOF. Following the neutron guide, first are choppers 1 & 2 which work together with 6 & 7 as velocity selector. Choppers 3 & 4 remove higher orders, 5 is the frame overlap chopper. The time needed for the neutrons to get from the sample to the detectors encodes their energy.

The primary spectrometer consists of seven rotating chopper discs which are placed in evacuated vessels (colored green on the cover page). The discs are made of carbon fiber composites and are coated with neutron-absorbing boron. On opposing sides, slits have been manufactured into the discs through which neutrons can pass. The first and last pair of choppers rotate in opposite direction each.

The incoming white neutron beam is pulsed by the first pair of choppers (choppers 1 and 2, pulsing choppers). This pulse still consists of neutrons with all velocities (or wavelength). Thus the pulse spreads along the way to the last chopper pair. These last two choppers (choppers 6 and 7, monochromating choppers) select a narrow range of wavelengths out of the pulse. The third and fourth chopper filter out higher orders (higher order removal choppers).

The fifth chopper is the frame overlap chopper. After the scattering process some neutrons fly towards the detectors, where they will be registered as a function of arrival time. It is essential that all scattered neutrons of one pulse are detected before the neutrons from the next pulse arrive. The overlap of slow neutrons from a pulse with fast neutrons of the following pulse inside the secondary spectrometer is called frame overlap. The frame-overlap-chopper blocks out several pulses, in order to avoid such an overlap.

The energy resolution (i.e. the width of the elastic line) is mainly determined by the chosen wavelength and the length of the neutron pulse that impinges on the sample. A good energy resolution can be achieved with a high rotational speed of the chopper discs (up to 22000 revolutions/minute). The energy resolution of the spectrometer can be changed continuously in the range from roughly $5 \mu\text{eV}$ to 5 meV (Fig. 3). By defining the energy uncertainty one can modify the time of observation in the range from roughly 1 ps to 1 ns.

The intensity of the incident neutron beam is recorded with a monitor, which is located between the primary spectrometer and the sample. An ionization chamber is used as a monitor, filled with fissile matter (^{235}U). The incoming neutrons trigger a fission and the high-energy nuclear fission products generate a clear voltage pulse, due to their high ionization density.

After passing the monitor, the neutrons hit the sample. Most of the neutrons are transmitted and are captured in the beamstop, but about 10 % of the neutrons are scattered in all possible directions. The neutrons that are scattered in the direction of the detector enter the flight chamber,

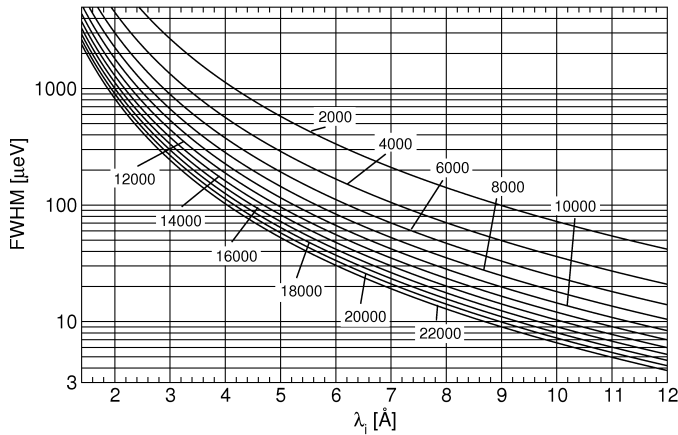


Fig. 3: Calculated energy resolution of the TOFTOF spectrometer shown for several chopper rotation speeds as function of the initial neutron wavelength. The chopper rotation speeds are given in rounds per minute (rpm) [4].

which occupies the space between the sample and detectors. The chamber is filled with argon in order to avoid unwanted scattering with air molecules.

Altogether 1000 ^3He -detectors (40 cm long and 3 cm in diameter) are placed tangential to the Debye-Scherrer-circles and also tangential to an imaginary spherical surface with a radius of 4 m around the position of the sample. Thus the flightpath from the sample to the detectors is 4 m long. The scattering angle 2θ covers a region from 7.5° to 140° . The detection of the scattered neutrons inside the ^3He -detectors occurs via a (n,p)-reaction. Hereby the neutrons are registered and tagged with a time stamp. The amount of detected neutrons is saved in time of flight bins for each detector in raw data files.

3 Theory

3.1 Cross sections

The probability that a neutron is scattered by a nucleus is denoted by the scattering cross section σ . It depends on:

1. the element
2. the isotope
3. the relative spin orientation of neutron and nucleus

Imagine a single crystal. The scattering cross section of every nucleus i can be decomposed into $\bar{\sigma} \pm \Delta\sigma_i$ where $\bar{\sigma}$ is the average over the whole crystal. This averaged part of the scattering cross section is called the *coherent scattering cross section*: scattered neutrons which can be

nuclide / element	σ_{coh} (barn)	σ_{inc} (barn)	σ_{abs} (barn)
^1H	1.758	80.27	0.3326
^2H	5.592	2.05	0.0005
H	1.760	80.26	0.3326
C	5.551	0.001	0.0035
N	11.01	0.5	11.51
O	4.232	0.001	0.0002
F	4.017	0.001	0.0096
Al	1.495	0.01	0.231
P	3.307	0.005	0.172
V	0.02	5.08	5.08

Table 1: Coherent and incoherent scattering cross sections as well as absorption cross sections of some selected nuclei or elements in their natural isotope composition, 1 barn = 100 fm². Source: [2].

described by this part of the scattering cross section “see” a regular lattice and interfere to a regular scattering pattern.

In contrast, the $\Delta\sigma$ are distributed randomly throughout the crystal and the scattering of the neutrons which can be described by the $\Delta\sigma$ does not interfere to a special pattern. This effect is attributed to an artificial quantity, the *incoherent scattering cross section*.

The proton (^1H) has the biggest incoherent cross section of all nuclei we study normally (about 80 barn, cf. Tab. 1). For practical purposes, the big difference between the incoherent scattering cross section of the proton and the deuteron (^2H) is of enormous importance. Using isotope exchange, i. e. (partial) deuteration of molecules, specific parts of the sample can be masked.

Vanadium scatters at the employed wavelengths also mainly incoherently although not as strong as the proton.

3.2 Principle of a scattering experiment

At a scattering experiment, two important values are recorded (cf. Fig. 4):

- The scattering vector \mathbf{Q} is defined as the difference between the wave vector \mathbf{k}_f of the scattered wave (f as “final”) and the wave vector \mathbf{k}_i of the incident wave (i as “initial”). The momentum gained or lost during the scattering process can be calculated by

$$\Delta\mathbf{p} = \hbar\mathbf{Q} = \hbar(\mathbf{k}_f - \mathbf{k}_i) . \quad (1)$$

However, the momentum transfer is commonly not noted. Instead, the scattering vector is commonly stated in units of inverse Ångstrom.

- The energy transfer ΔE is defined as the energy of the neutron after E_f and before E_i the

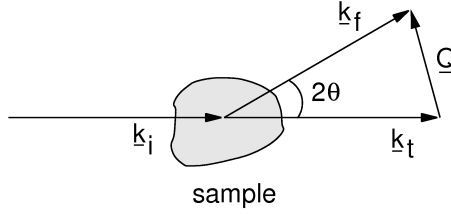


Fig. 4: Schematic representation of a scattering experiment. $\mathbf{k}_{i,f,t}$ are the wave vectors of the initial (incoming), final (scattered) and transmitted neutrons, respectively. \mathbf{Q} is the scattering vector.

scattering process:

$$\Delta E = \hbar\omega = \hbar(\omega_f - \omega_i) = \frac{\hbar^2(|\mathbf{k}_f|^2 - |\mathbf{k}_i|^2)}{2m_n}. \quad (2)$$

The energy transfer is measured in meV. Often, ω is written incorrectly instead of $\hbar\omega$.

The absolute value of the wave vectors \mathbf{k} is defined as $|\mathbf{k}| = 2\pi/\lambda$, with an refractive index $n \approx 1$ (which is a very good approximation for neutrons). However, the scattering vector cannot be measured directly, only the wave vector of the incident and scattered neutrons. Using the law of cosine one obtains a general equation for converting k_i and k_f to Q :

$$|\mathbf{Q}|^2 = |\mathbf{k}_i|^2 + |\mathbf{k}_f|^2 - 2|\mathbf{k}_i||\mathbf{k}_f|\cos(2\theta). \quad (3)$$

In the case of elastic scattering, the energy transfer is zero. Hence $|\mathbf{k}_i| = |\mathbf{k}_f|$ simplifies the equation to

$$Q = \frac{4\pi}{\lambda} \sin\left(\frac{2\theta}{2}\right) \quad (4)$$

where $Q = |\mathbf{Q}|$. Roughly speaking a distance d in direct space corresponds to a Q value

$$Q = \frac{2\pi}{d}. \quad (5)$$

Therefore one can extract information about the physical configuration of the nuclei in the sample by analyzing the intensity of the elastic scattering as a function of Q (the diffractogram), cf. Fig. 6. Furthermore the intensity at a certain value of Q as a function of energy (a spectrum) provides information about the motion of the nuclei (see Fig. 6).

3.3 Correlation & scattering functions

The position and the motions of the nuclei in any system can be described using correlation functions. It can be shown that these correlation functions are what is measured with scattering methods.

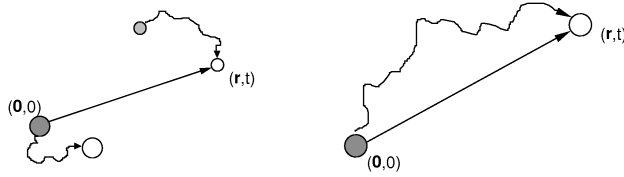


Fig. 5: Left: Pair correlation, right: self correlation. In the case of pair correlation, the second particle may be a different one than the first one but it doesn't have to.

The *pair correlation function* $G_{\text{pair}}(\mathbf{r}, t)$ gives the probability to find a particle j at time t at the place \mathbf{r} if this or another particle i was at time $t = 0$ at the origin $\mathbf{r} = \mathbf{0}$, as shown in Fig. 5. The pair correlation function is

$$G_{\text{pair}}(\mathbf{r}, t) = \frac{1}{N} \sum_{i=1}^N \sum_{j=1}^N \int \langle \delta\{\tilde{\mathbf{r}} - \mathbf{R}_i(0)\} \cdot \delta\{\tilde{\mathbf{r}} + \mathbf{r} - \mathbf{R}_j(t)\} \rangle d\tilde{\mathbf{r}}, \quad (6)$$

with the number of particles N , an integration variable $\tilde{\mathbf{r}}$ and the place $\mathbf{R}_j(t)$ of particle j at time t . The angle brackets $\langle \rangle$ denote an ensemble average.

The *self correlation function* or *auto correlation function* $G_{\text{self}}(\mathbf{r}, t)$ gives the probability to find one particle at time t at place \mathbf{r} if this very particle was at time $t = 0$ at the place $\mathbf{r} = \mathbf{0}$, see again Fig. 5. It is defined as

$$G_{\text{self}}(\mathbf{r}, t) = \frac{1}{N} \sum_{i=1}^N \int \langle \delta\{\tilde{\mathbf{r}} - \mathbf{R}_i(0)\} \cdot \delta\{\tilde{\mathbf{r}} + \mathbf{r} - \mathbf{R}_i(t)\} \rangle d\tilde{\mathbf{r}}. \quad (7)$$

In the following, we will assume that the samples are powder samples or liquids (i. e. not single crystals) and will therefore use the absolute value of \mathbf{r} , r , instead of the vector.

It is possible to calculate the pair and self correlation function from the scattered intensities. Roughly, the calculation is as follows:

From the intensity of the scattered neutrons measured as function of momentum and energy change, one obtains the *double differential scattering cross section* which can be seen as the sum of a coherent and an incoherent part:

$$\frac{d^2\sigma}{d\Omega dE'} = \frac{k_f}{k_i} \frac{N}{4\pi} (\sigma_{\text{coh}} S_{\text{coh}}(Q, \omega) + \sigma_{\text{inc}} S_{\text{inc}}(Q, \omega)). \quad (8)$$

It denotes the probability that a neutron is scattered into the solid angle $d\Omega$ with an energy change dE' . N is the number of scattering nuclei and $S(Q, \omega)$ is called the *scattering function*.

The Fourier transform in time and space of the coherent scattering function $S_{\text{coh}}(Q, \omega)$ is nothing but the pair correlation function $G_{\text{pair}}(r, t)$ and the Fourier transform in time and space of $S_{\text{inc}}(Q, \omega)$ is the self correlation function $G_{\text{self}}(r, t)$.

Three functions are important:

1. the *correlation function* $G(r, t)$
2. the *intermediate scattering function* $I(Q, t)$ which is the Fourier transform (from r to Q) of $G(r, t)$
3. the *scattering function* $S(Q, \omega)$ which is the Fourier transform (from t to ω) of $I(Q, t)$

All of them exist in two versions, considering pairs of particles (pair correlation function) or only one particle (self correlation function).

For the intermediate scattering function $I(\mathbf{Q}, t)$ one can obtain further expressions – for a pair correlation

$$I_{\text{coh}}(\mathbf{Q}, t) = \frac{1}{N} \sum_{i=1}^N \sum_{j=1}^N \langle e^{-i\mathbf{Q}\mathbf{R}_i(0)} e^{i\mathbf{Q}\mathbf{R}_j(t)} \rangle \quad (9)$$

and for the self correlation function

$$I_{\text{inc}}(\mathbf{Q}, t) = \frac{1}{N} \sum_{i=1}^N \langle e^{-i\mathbf{Q}\mathbf{R}_i(0)} e^{i\mathbf{Q}\mathbf{R}_i(t)} \rangle . \quad (10)$$

At neutron spin echo spectrometers, the intermediate scattering function is measured – all other neutron scattering spectrometers, including TOFTOF, measure the scattering function.

At TOFTOF, we mainly probe the non-periodic motions in disordered materials, for instance diffusion processes in liquids. If a scatterer performs several motions simultaneously (but independently from each other), the resulting incoherent scattering function is a convolution in energy space of the single scattering functions, for example

$$S_{\text{total}}(Q, \omega) = S_{\text{diffusion}}(Q, \omega) \otimes S_{\text{internal motion}}(Q, \omega) . \quad (11)$$

As a convolution corresponds to a multiplication after Fourier transform, one can also write

$$I_{\text{total}}(Q, t) = I_{\text{diffusion}}(Q, t) \cdot I_{\text{internal motion}}(Q, t) . \quad (12)$$

If two scatterers perform two motions independently from each other and both cause incoherent scattering, the recorded total incoherent scattering function is simply the sum of the two scattering functions, for example

$$S_{\text{total}}(Q, \omega) = S_{\text{solute}}(Q, \omega) + S_{\text{solvent}}(Q, \omega) , \quad (13)$$

which is also a sum after Fourier transform to the intermediate scattering function.

This decomposition of the scattering functions into parts is *very* important.

Due to the limited number of supporting points it is not possible to obtain the correlation function by numerical Fourier transform of the measured scattering function. Therefore, one proceeds the other way round: After inventing a plausible correlation function, one performs a Fourier transform of this theoretical function to a scattering function and checks if this can describe the data.

The hereby obtained theoretical scattering function $S_{\text{theor}}(Q, \omega)$ is fitted to the measured scattering function $S_{\text{meas}}(Q, \omega)$ after convolving the theoretical scattering function with the measured instrumental resolution. The instrumental resolution is often determined using a vanadium sample which is an elastic, incoherent scatterer.

4 Experiment

4.1 The system

In this experiment we will study the diffusive motions of molecules, e.g. *n*-alkanes or salt solutions. By analyzing this system we want to learn more about the mechanism of molecular self-diffusion, i.e. internal motions of the molecules and long-range diffusion processes.

4.2 Modelling the motions

Molecules in general are by far too complex to come up with a scattering function which describes all the motions correctly. Therefore, very simplified models are used. Assuming that the molecule itself is rigid and moves as a whole, one obtains the scattering function

$$S_{\text{diffusion}}(Q, \omega) = \frac{1}{\pi} \frac{|\Gamma_d(Q)|}{\omega^2 + \Gamma_d(Q)^2}, \quad (14)$$

a Lorentzian with a Q -dependent width $|\Gamma_d(Q)|$. If the diffusion follows exactly Fick's law, one obtains

$$|\Gamma_d(Q)| = D \cdot Q^2 \quad (15)$$

with the diffusion coefficient D which is normally given in m^2/s .

Deviations from this ideal $\propto Q^2$ law indicate that the observed process is not ideal Fick diffusion. A constant (too large) value of Γ_d at small Q can be a sign of *confinement*: the molecule cannot escape from a cage formed by the neighbouring molecules. If the width Γ_d goes towards a constant value at large Q , this can be a sign of *jump diffusion* which should rather be named *stop-and-go diffusion*: the molecule sits for some time at a certain place, then diffuses for a while, gets trapped again, ...

Try to fit the data with one Lorentzian. If this model does not describe the data satisfactorily, the assumption of a rigid molecule was probably not justified. The scattering function for a localized motion can be written as:

$$S_{\text{intern}}(Q, \omega) = A_0(Q) \cdot \delta(\omega) + (1 - A_0(Q)) \cdot \frac{1}{\pi} \frac{|\Gamma_i|}{\omega^2 + \Gamma_i^2}, \quad (16)$$

that is the sum of a delta-function and a Lorentzian (confer also figure 6). $|\Gamma_i|$ gives the frequency of the motion, $A_0(Q)$ is called the *elastic incoherent structure factor* (EISF) and it gives information on the long time average position of the scatterer, in first approximation the size of the localized motion.

As we assume that the molecule performs a local motion and long-range diffusion simultaneously but independently from each other, we have to convolve the two functions with each other. The result is the sum of two Lorentzians:

$$S(Q, \omega) = F(Q) \cdot \left\{ \frac{A_0(Q)}{\pi} \frac{|\Gamma_d(Q)|}{\omega^2 + \Gamma_d(Q)^2} + \frac{1 - A_0(Q)}{\pi} \frac{|\Gamma_d(Q)| + |\Gamma_i|}{\omega^2 + (|\Gamma_d(Q)| + |\Gamma_i|)^2} \right\}. \quad (17)$$

4.3 The experiment itself

We might either produce a sample together or fill an existing sample into the aluminium hollow cylindrical container or a flat aluminium container. This sample is then measured at TOFTOF, additionally a vanadium standard and the empty aluminum container will be measured. The length and number of measurements will have to be adjusted to the available time, it will be necessary to use some measurements of the preceding groups.

You will do all sample changes in the presence of a tutor who explains the procedure in detail.

4.4 Data reduction

The instrument saves the number of counts as a function of scattering angle and time-of-flight, $N(2\theta, \text{tof})$. The next step is the data reduction which applies several corrections and transforms to get rid of many instrument-specific properties of the data and convert them to a scattering function $S(Q, \omega)$.

Data reduction (and later on also data evaluation) is done using the program LAMP [5]. On the Desktop launch the icon “LAMP”. LAMP is used in many large scale facilities and it includes a variety of different instrument routines. To start the program, in the main window upper part, the working `Path` has to be set: just enter the folder path where you will work and create output files. Then you need to choose the instrument where you are working, in this case search for “`toftof`”.

LAMP is structured in “workspaces”. A workspace contains all necessary data like the time of flight/energy transfer of the neutron, its $2\theta/Q$ - values and the Intensity. It can also contain information about the measurement settings or sample conditions (e.g. temperature). Any operation on the data takes as an input a workspace and the output is stored in another workspace `w1`, `w2`, etc...(pay attention to not overwrite workspaces during the data reduction). A list of commands used to reduce data can be found in the manual [5] and in the TOF Data Reduction [6].

Raw data files that have been measured under the same conditions (e.g. temperature) can be added and treated as one data set. This will be done in the loading routine. After reading the data files, the raw data $N(2\theta, \text{tof})$ are normalized to the incoming neutron flux. The empty can measurement is subtracted from the data and the sensitivity of each detector is calibrated using the vanadium standard measurement. As vanadium is an incoherent scatterer, it should scatter the same intensity in all directions. The only effect which causes deviations from an isotropic scattering is the Debye-Waller-factor (DWF) which is well-known and can be corrected. This is followed by the calculation of the energy transfer from the time-of-flight so that one obtains $S(2\theta, \omega)$.

The next step is to calculate the momentum transfer Q from the scattering angle 2θ and the energy transfer ω using equation (3). During this step, we obtain about 1000 spectra with relatively low statistics each and a varying value of Q as the energy transfer varies. To get a better statistics and to have spectra which have the same Q for all values of energy transfer, the 1000 spectra are grouped into about n spectra of constant ΔQ in the same routine. A typical reduction routine is given in table 4.4.

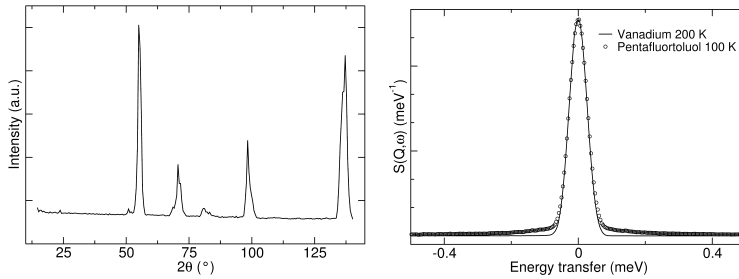


Fig. 6: Left: Neutron diffraction patterns of solid pentafluorotoluene at 100 K ($\lambda_i = 6 \text{ \AA}$), taken from [3]. If the scattering vector is a reciprocal lattice vector, the positive interference of neutron waves yields a maximum in the scattered intensity. The sharp features in the diffraction pattern indicate an ordered lattice. Right: The spectra $S(Q, \omega)$ of pentafluorotoluene (\circ) and vanadium (—) at a momentum transfer of $Q = 1.1 \text{ \AA}^{-1}$, cf. also [3]. The solid sample shows only an internal motion, can therefore be described by equation 16.

```

w1 = rdsum('File1', 'FileEnd')           ; Read sample runs
w1 = normalise(w1, /monitor)              ; Normalize to monitor
w2 = rdsum('FileEC1', 'FileECEnd')       ; Read empty run
w2 = normalise(w2, /monitor)
w3 = w1 - w2                             ; Subtract the background
e3 = sqrt(e1^2 + e2^2)                   ; Propagate the errors
w20 = rdsum('FileVan1', 'FileVanEnd')    ; read vanadium run
w20 = normalise(w20, /monitor)
w4 = vnorm(w3, w20, min = 500 , max = 600 ) ; Normalize w3 to vanadium
                                           ; spectra, integrated around
                                           ; the elastic channel
w5 = remove_spectra(w4, [1,2,3,4])       ; Remove noisy detectors
w6 = t2e(w5)                             ; Convert from tof to energy
w7 = reb(w6, dE = 0.1)                   ; Rebin energy at constant dE
w8 = sqw_rebin(w7, dQ = 0.1 , emin = -5) ; Rbin to S(Q,w) with a
                                           ; given dQ binning.

```

Table 2: Typical data reduction routine for TOFTOF.

4.5 Data evaluation

For a quantitative analysis, fit the spectra with the functions given in section 4.2. For this purpose, a fit-routine in LAMP can be used: menu `TOOLS` → `FITTING` with `STRfit`. As the theoretical functions have to be convolved with the experimental resolution, the program will ask for the converted and grouped spectra of vanadium.

The numbers shown in lower part of the window are the reduced χ^2 , which is a measure for the quality of the fit, and the fitted values of the parameters. Judge the fit quality by the reduced χ^2 and by visually inspecting the fits together with the data. Plot the obtained parameters for the width, Γ , as function of Q^2 and determine the diffusion coefficient.

If you measured the sample at different temperatures, repeat the procedure for all of them.

5 Questions to be answered *before* the experiment

1. Do you expect the vanadium sample to be activated by the neutron beam? What about the aluminium container with the real sample? (2 min)
2. The vanadium standard sample at TOFTOF is a hollow cylinder with an outer diameter of 22.5 mm and a height of 65 mm. The wall thickness is 0.6 mm. Which fraction of the neutrons that hit the vanadium will be scattered? How big is the transmission?
3. Why do the samples measured at TOFTOF mostly have a transmission of about 90 %? How can the transmission be adjusted? (3 min)
4. The substance to be measured is filled in a gap between the inner and the outer cylinder of the sample container. The inner diameter of the outer cylinder is always 22.5 mm, the inner cylinder can be chosen to have either 22.1 mm or 22.3 mm outer diameter. The height of the cylinders is 65 mm. How large is the sample volume for the two different inner cylinders? Which inner cylinder would you use? (5 min)
5. Please note where this handout could need improvement. (5 min)

6 Questions to be answered *during* the experiment

1. When measuring water-based samples, H_2O is most often replaced by D_2O when the water is not the subject of the study. Why? The signal of the solvent has to be subtracted in both cases! (2 min)
2. Why is the sample container made of aluminum? (2 min)
3. The Vanadium standard sample at TOFTOF (hollow cylinder, 2 cm outer diameter, 0.6 mm thickness) is a “7% scatterer”, meaning that it transmits 93% of the neutrons. In the moment, TOFTOF has 1000 neutron detectors with an active area of 40x3 cm each in 4 m distance from the sample. Estimate the efficiency of the monitor detector using the *Monitor rate* and *Signal Rate* given by the control program. (5 min)

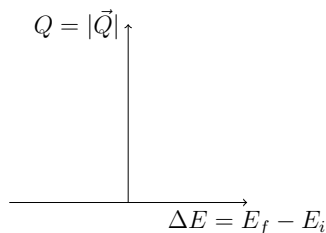


Fig. 7: *Dynamic range plot.*

4. To calculate the energy of neutrons in meV with a well-known wavelength given in Å, one can use a formula

$$E \approx \frac{a}{\lambda^2}. \quad (18)$$

Determine a numerical value for a . How big is the initial energy E_i of the neutrons in the current experiment? (5 min)

5. What is the maximal energy transfer from the neutron to the sample? (1 min)
6. What is the maximal energy transfer from the sample to the neutron? (1 min)
7. Draw at least six scattering triangles (as shown in Fig. 4) for these points in the dynamical range:

- Elastic scattering with a scattering angle of 7.5° ; with a scattering angle of 140° (the first & last detector at TOFTOF)
- Same scattering angles with neutron energy gain
- Same scattering angles with neutron energy loss

(6 min)

8. Locate those points in this dynamic range plot and determine which area in this plot is accessible in the current scattering experiment. (5 min)
9. How can you distinguish coherent and incoherent scattering in the diffraction pattern? Which information can you extract from the spectra when they are caused by coherent or incoherent scattering, respectively? (2 min)
10. Why do we measure Vanadium? (three reasons; for one it is important that Vanadium scatters neutrons incoherently, for two it is important that the Vanadium signal does not have a quasielastic broadening) (6 min)
11. Assume that the scatterers in your sample are partially trapped. They diffuse inside a “cage” until they find a hole through which they can escape. How do the intermediate scattering function $I(Q, t)$ and the scattering function $S(Q, \omega)$ look like? (5 min)

7 Constants

$$m_n = 1.675 \cdot 10^{-27} \text{ kg} \tag{19}$$

$$h = 6.626 \cdot 10^{-34} \text{ J} \cdot \text{s} = 4.136 \cdot 10^{-15} \text{ eV} \cdot \text{s} \tag{20}$$

$$\hbar = 1.055 \cdot 10^{-34} \text{ J} \cdot \text{s} = 6.582 \cdot 10^{-16} \text{ eV} \cdot \text{s} \tag{21}$$

$$e = 1.602 \cdot 10^{-19} \text{ C} \tag{22}$$

References

- [1] S. König, W. Pfeiffer, T. Bayerl, D. Richter, and E. Sackmann, *Journal de Physique II* **2**, 1589 (1992).
- [2] National Institute of Standards and Technology, “Neutron scattering lengths and cross sections” (1992) <http://www.ncnr.nist.gov/resources/n-lengths/list.html>.
- [3] C. Smuda, G. Gemmecker, and T. Unruh, *Journal of Chemical Physics* **128**, 194502 (2008).
- [4] T. Unruh, Jürgen Neuhaus, and Winfried Petry, *Nucl. Instrum. Methods Phys. Res. A* **580**, 1414 (2007).
- [5] LAMP, the Large Array Manipulation Program www.ill.eu/data_treat/lamp/the-lamp-book/.
- [6] TOF Data Reduction (ILL) <https://www.ill.eu/instruments-support/instruments-groups/groups/tof/software/tof-lamp/tof-reduction/>.

Contact

TOFTOF

Phone: 089/289-14881

Web: <http://www.mlz-garching.de/instrumente/spektroskopie/toftof.html>

Wiebke Lohstroh

Forschungsneutronenquelle Heinz Maier-Leibnitz (FRM II)
und Physik Department E13
Technische Universität München

Phone: 089/289-14735

e-Mail: wiebke.lohstroh@frm2.tum.de

Luca Silvi

Phone: 089/289-14922

e-Mail: luca.silvi@frm2.tum.de

Band / Volume 94

Functional Soft Matter

Lecture Notes of the 46th IFF Spring School 2015

23 February – 06 March, 2015 Jülich, Germany

ed. by J. Dhont, G. Gompfer, G. Meier, D. Richter, G. Vliegenthart, R. Zorn
(2015), ca. 600 pp

ISBN: 978-3-89336-999-7

Band / Volume 95

**2-Steps in 1-pot: enzyme cascades for the synthesis
of chiral vicinal amino alcohols**

T. Sehl (2014), XIV, 167 pp

ISBN: 978-3-95806-001-2

Band / Volume 96

**Immunohistochemical and electrophysiological characterization of the
mouse model for Retinitis Pigmentosa, *rd10***

S. Biswas (2014), XII, 119 pp

ISBN: 978-3-95806-011-1

Band / Volume 97

**Single molecule localization microscopy: Imaging of cellular structures
and a new three-dimensional localization technique**

X. Fan (2014), XII, 92 pp

ISBN: 978-3-95806-014-2

Band / Volume 98

Cryogenic Break-Junction Characterization of Single Organic Molecules

T. Grellmann (2014), VI, 86 pp

ISBN: 978-3-95806-015-9

Band / Volume 99

**Interacting Interactions: A Study on the Interplay of Molecule-Molecule
and Molecule-Substrate Interactions at Metal-Organic Interfaces**

M. Willenbockel (2014), IX, 245 pp

ISBN: 978-3-95806-018-0

Band / Volume 100

**Microwire crossbar arrays for chemical, mechanical,
and thermal stimulation of cells**

P. Rinklin (2015), xii, 184 pp

ISBN: 978-3-95806-022-7

Band / Volume 101

Modification and characterization of potential bioelectronic interfaces

K. Greben (2015), 76 pp

ISBN: 978-3-95806-028-9

Band / Volume 102

Extending the precision and efficiency of the all-electron full-potential linearized augmented plane-wave density-functional theory method

G. Michalíček (2015), 195 pp

ISBN: 978-3-95806-031-9

Band / Volume 103

Metabolic engineering of *Escherichia coli* for the production of plant phenylpropanoid derived compounds

P. V. van Summeren-Wesenhagen (2015), V, 92 pp

ISBN: 978-3-95806-039-5

Band / Volume 104

Spin-reorientation transition in epitaxial $\text{Ni}_x\text{Pd}_{1-x}$ films on Cu(001): a microscopic analysis

D. Gottlob (2015), x, 134 pp

ISBN: 978-3-95806-049-4

Band / Volume 105

Resonant Magnetic Scattering Studies using Synchrotron Radiation and Laser-Generated Extreme Ultraviolet Light

C. M. Weier (2015), vii, 143 pp

ISBN: 978-3-95806-052-4

Band / Volume 106

Neutron Scattering

Lectures of the JCNS Laboratory Course held at Forschungszentrum Jülich and at the Heinz-Maier-Leibnitz Zentrum Garching

edited by Th. Brückel, D. Richter, G. Roth, A. Wischnewski and R. Zorn (2015), ca 300 pp

ISBN: 978-3-95806-055-5

Band / Volume 107

Neutron Scattering

Experiment Manual of the JCNS Laboratory Course held at

Forschungszentrum Jülich and at the Heinz-Maier-Leibnitz Zentrum Garching

edited by Th. Brückel, D. Richter, G. Roth, A. Wischnewski and R. Zorn (2015), ca 150 pp

ISBN: 978-3-95806-056-2

Weitere **Schriften des Verlags im Forschungszentrum Jülich** unter

<http://www.zb1.fz-juelich.de/verlagextern1/index.asp>

Schlüsseltechnologien /
Key Technologies
Band / Volume 107
ISBN 978-3-95806-056-2

